



# OMU 408

---

## 4/8 CHANNEL DATA LOGGER

DC VOLTMETER/AMMETER

PROCESS MONITOR

OHMMETER

THERMOMETER FOR PT 100/500/1 000

THERMOMETER FOR NI 1 000

THERMOMETER FOR THERMOCOUPLES

DISPLAY UNIT FOR LIN. POTENTIOMETERS



## **SAFETY INSTRUCTIONS**

Please, read the enclosed safety instructions carefully and observe them!  
These instruments should be safeguarded by isolated or common fuses (breakers)!  
For safety information the EN 61 010-1 + A2 standard must be observed.  
This instrument is not explosion-safe!

## **TECHNICAL DATA**

Measuring instruments of the O MU 408 series conform to the European regulation 89/336/EWG and the Ordinance 168/1997 Coll.

The instruments are up to the following European standards:

EN 55 022, class B

EN 61000-4-2, -4, -5, -6, -8, -9, -10, -11

The instruments are applicable for unlimited use in agricultural and industrial areas.

## **CONNECTION**

Supply of energy from the main line has to be isolated from the measuring leads.



## **ORBIT MERRET, spol. s r.o.**

Vodňanská 675/30

198 00 Prague 9

Czech Republic

Tel: +420 - 281 040 200

Fax: +420 - 281 040 299

e-mail: [orbi@merret.cz](mailto:orbi@merret.cz)

[www.orbit.merret.cz](http://www.orbit.merret.cz)



1.	Contents .....	3
2.	Instrument description .....	4
3.	Instrument connection .....	6
4.	Instrument setting .....	8
	Symbols used in the instructions .....	10
	Setting the DP and the (-) sign .....	10
	Control keys function .....	11
	Setting/permitting items into "USER" menu .....	11
5.	Setting "LIGHT" menu .....	12
5.0	Description "LIGHT" menu .....	12
	Setting input - Type "DC" .....	16
	Setting input - Type "PM" .....	18
	Setting input - Type "DU" .....	20
	Setting input - Type "OHM" .....	22
	Setting input - Type "RTD - Pt" .....	24
	Setting input - Type "RTD - Cu" .....	26
	Setting input - Type "RTD - Ni" .....	28
	Setting input - Type "T/C" .....	30
	Setting Limits .....	32
	Setting analog output .....	34
	Selection of programming menu „LIGHT“/„PROFI“ .....	36
	Restoration of manufacture setting .....	36
	Calibration - input range (DU) .....	37
	Selection of instrument menu language version .....	38
	Setting new access password .....	38
	Instrument identification .....	39
6.	Setting "PROFI" menu .....	40
6.0	Description of "PROFI" menu .....	40
6.1	"PROFI" menu - INPUT .....	42
6.1.1	Resetting internal values .....	42
6.1.2	Setting measuring type, range, mode, rate, .....	43
6.1.3	Setting the Real Time .....	51
6.1.4	External input function selection .....	52
6.1.5	Optional accessory functions of the keys .....	53
6.2	"PROFI" menu - CHANNEL .....	58
6.2.1	Setting measuring parameters (projection, filters, decimal point, description) .....	58
6.2.2	Setting mathematic functions .....	63
6.2.3	Selection of evaluation of min/max. value .....	67
6.3	"PROFI" menu - OUTPUT .....	68
6.3.1	Setting data logging .....	70
6.3.2	Setting Limits .....	73
6.3.3	Setting data output .....	74
6.3.4	Setting analog output .....	76
6.4	"PROFI" menu - SERVICE .....	78
6.4.1	Selection of programming menu „LIGHT“/„PROFI“ .....	79
6.4.2	Restoration manufacture setting .....	79
6.4.3	Calibration - input range (DU) .....	80
6.4.4	Selection of instrument menu language version .....	80
6.4.5	Setting new access password .....	81
6.4.6	Instrument identification .....	81
7.	Setting items into "USER" menu .....	82
8.	Method of measuring of the cold junction .....	84
9.	Data protocol .....	86
10.	Error statements .....	88
11.	Table of symbols .....	89
12.	Technical data .....	90
13.	Instrument dimensions and instalation .....	92
14.	Certificate of guarantee .....	93

## 2.1 Description

The OMU 408 is a 4/8 channel data logger, designed for maximum purposefulness and user comfort while maintaining its low cost. It is a multifunction instrument with the option of configuration for 8 different types of input, easily configurable in the menu.

The instrument is based on an 8-bit microprocessor with multi-channel 24-bit sigma-delta converter, which ensures the instrument high accuracy, stability and easy operation.

Major advantage of the instrument is with respect to the high rate of sampling on individual channels the feasibility to evaluate all measuring inputs simultaneously.

### **The OMU 408UNI is a multifunction instrument available in following types and ranges**

<b>DC:</b>	0...60/150/300/1200 mV
<b>PM:</b>	0...5 mA/0...20 mA/4...20 mA/ $\pm$ 2 V/ $\pm$ 5 V/ $\pm$ 10 V/ $\pm$ 40 V
<b>OHM:</b>	0...100 $\Omega$ /0...1 k $\Omega$ /0...10 k $\Omega$ /0...100 k $\Omega$
<b>RTD-Pt:</b>	Pt 50/100/Pt 500/Pt 1 000
<b>RTD-Cu:</b>	Cu 50/Cu 100
<b>RTD-Ni:</b>	Ni 1 000/Ni 10 000
<b>T/C:</b>	J/K/T/E/B/S/R/N
<b>DU:</b>	Linear potentiometer (min. 500 $\Omega$ )

### **PROGRAMMABLE PROJECTION**

Selection:	of type of input and measuring range
Measuring range:	adjustable as fixed
Setting:	manual, optional projection on the display may be set in the menu for both limit values of the input signal, e.g. input 0...20 mA > 0...850,0
Projection:	-999...9999

### **COMPENSATION**

of conduct:	in the menu it is possible to perform compensation for 2-wire connection
of conduct in probe:	internal connection (conduct resistance in measuring head)
of CJC (T/C):	manual or automatic, in the menu it is possible to perform selection of the type of thermocouple and compensation of cold junctions, which is adjustable or automatic (temperature at the brackets)

### **LINEARIZATION**

Linearization:*	by linear interpolation in 254 points (solely via OM Link)
-----------------	--

### **DIGITAL FILTERS**

Floating average:	from 2...30 measurements
Exponen.average:	from 2...100 measurements
Rounding:	setting the projection step for display

### **MATHEMATIC FUCNTIONS**

Min/max. value:	registration of min./max. value reached during measurement
Tare:	designed to reset display upon non-zero input signal
Peak value:	the display shows only max. or min. value
Mat. operations:	polynome, 1/x, logarithm, exponential, power, root, sin x and mathematic operatin between input - total, divergence, divide

\* only for type DC, PM, DU

**EXTERNAL CONTROL**

Lock:	control keys blocking
Hold:	display/instrument blocking
Tare:	tare activation/resetting tare to zero
Resetting MM:	resetting min/max value
Memory:	data storage into instrument memory

**2.2 Operation**

The instrument is set and controlled by five control keys located on the front panel. All programmable settings of the instrument are performed in three adjusting modes:

**LIGHT Simple programming menu**

- contains solely items necessary for instrument setting and is protected by optional number code

**PROFI Complete programming menu**

- contains complete instrument menu and is protected by optional number code

**USER User programming menu**

- may contain arbitrary items selected from the programming menu (LIGHT/PROFI), which determine the right (see or change)
- access without password

All programmable parameters are stored in the EEPROM memory (they hold even after the instrument is switched off).



Complete instrument operation and setting may be performed via OM Link communication interface, which is a standard equipment of all instruments.

The operation program is freely accessible ([www.orbit.merret.cz](http://www.orbit.merret.cz)) and the only requirement is the purchase of OML cable to connect the instrument to PC. It is manufactured in version RS 232 and USB and is compatible with all ORBIT MERRET instruments. Another option for connection is with the aid of data output RS 232 or RS 485 (without the need of the OML cable).

The program OM LINK in „Basic“ version will enable you to connect one instrument with the option of visualization and archiving in PC. The OM Link „Standard“ version has no limitation of the number of instruments connected.

**2.3 Options**

**Comparators** are assigned to monitor one, two, three or four limit values with relay output. The user may select limits regime: LIMIT/DOSING/FROM-TO. The limits have adjustable hysteresis within the full range of the display as well as selectable delay of the switch-on in the range of 0...99,9 s. Reaching the preset limits is signalled by LED and simultaneously by the switch-on of the relevant relay.

**Data outputs** are for their rate and accuracy suitable for transmission of the measured data for further projection or directly into the control systems. We offer an isolated RS232 and RS485 with the ASCII or DIN MessBus protocol.

**Analog outputs** will find their place in applications where further evaluating or processing of measured data is required in external devices. We offer universal analog output with the option of selection of the type of output - voltage/current. The value of analog output corresponds with the displayed data and its type and range are selectable in Menu.

**Measured data record** is an internal time control of data collection. It is suitable where it is necessary to register measured values. Two modes may be used. FAST is designed for fast storage (40 records/s) of all measured values up to 8 000 records. Second mode is RTC, where data record is governed by Real Time with data storage in a selected time segment and cycle. Up to 250 000 values may be stored in the instrument memory. Data transmission into PC via serial interface RS232/485 and OM Link.


The instrument supply leads should not be in proximity of the incoming low-potential signals.  
Contactors, motors with larger input power should not be in proximity of the instrument.

The leads into the instrument input (measured quantity) should be in sufficient distance from all power leads and appliances.  
Provided this cannot be secured it is necessary to use shielded leads with connection to ground (bracket E).

The instruments are tested in compliance with standards for use in industrial area, yet we recommend to abide by the above mentioned principles.

### MEASURING RANGES

Type	Input I	Input U
DC	0...60/150/300/1 200 mV	
PM	0...5/20 mA/4...20 mA	±2/±5/±10/±40 V
OHM	0...0,1/1/10/100 kΩ	
RTD-Pt	Pt 100/Pt 500/ Pt 1 000	
RTD-Cu	Cu 50/100	
RTD-Ni	Ni 1 000/10 000	
T/C	J/K/T/E/B/S/R/N/L	
DU	Linear potentiometer (min. 500 Ω)	

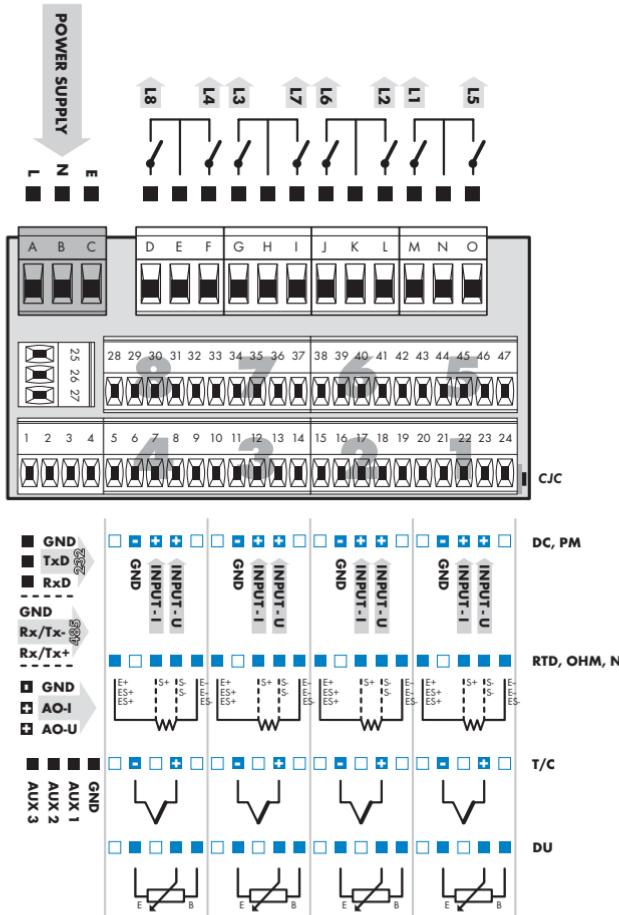

PROFI

The Profi logo consists of the word "profi" in a stylized, italicized font. The letters have a soft, glowing effect with highlights and shadows.

SETTING

The Light logo consists of the word "light" in a stylized, italicized font. The letters have a soft, glowing effect with highlights and shadows.

LIGHT

USER

The User logo consists of the word "user" in a bold, italicized font. The letters have a soft, glowing effect with highlights and shadows. Above the "user" logo, there is a small graphic element consisting of two overlapping semi-circles, one light blue and one light green.

SETTING

- ▶ • For expert users
- Complete instrument menu
- Access is password protected
- Possibility to arrange items of the „User“ menu
- Tree menu structure

- ▶ • For trained users
- Only items necessary for instrument setting
- Access is password protected
- Possibility to arrange items of the „User“ menu
- Linear menu structure

- ▶ • For user operation
- Menu items are set by the user (Profi/Light) as per request
- Access is not password protected
- Optional menu structure either tree (PROFI) or linear (LIGHT)

## 4.1 Setting

The instrument is set and controlled by five control keys located on the front panel. All programmable settings of the instrument are performed in three adjusting modes:

### LIGHT Simple programming menu

- contains solely items necessary for instrument setting and is protected by optional number code

### PROFI Complete programming menu

- contains complete instrument menu and is protected by optional number code

### USER User programming menu

- may contain arbitrary items selected from the programming menu (LIGHT/PROFI), which determine the right (see or change)
- access without password


All programmable parameters are stored in the EEPROM memory (they hold even after the instrument is switched off).

Complete instrument operation and setting may be performed via OM Link communication interface, which is a standard equipment of all instruments.


The operation program is freely accessible ([www.orbit.merret.cz](http://www.orbit.merret.cz)) and the only requirement is the purchase of OML cable to connect the instrument to PC. It is manufactured in version RS 232 and USB and is compatible with all ORBIT MERRET instruments.

Another option for connection is with the aid of data output RS 232 or RS 485 (without the need of the OML cable).

### Scheme of processing the measured signal

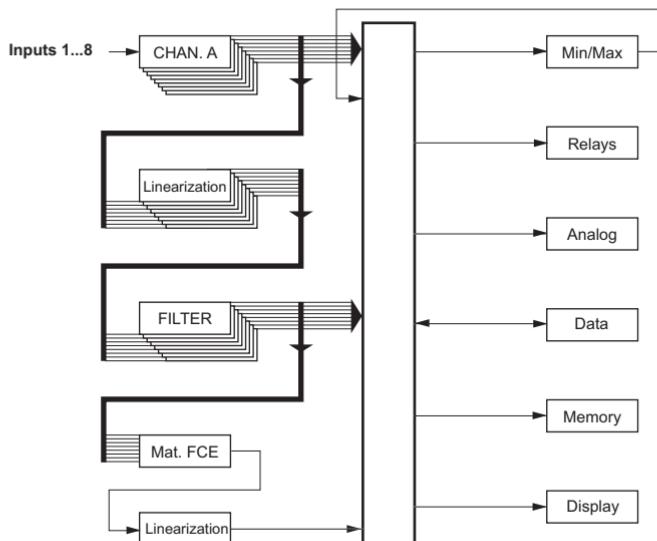

Setting and controlling the instrument is performed by means of 5 control keys located on the front panel. With the aid of these keys it is possible to browse through the operation menu and to select and set required values.

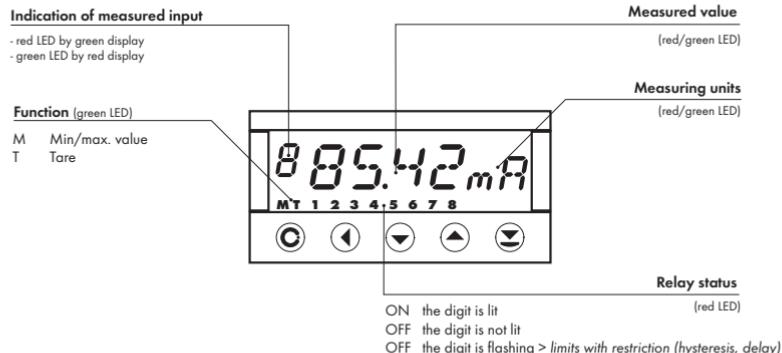

#### Symbols used in the instructions

**DC PM**  
**DU OHM RTD T/C** Indicates the setting for given type of instrument

**DEF** values preset from manufacture

symbol indicates a flashing light (symbol)

inverted triangle indicates the item that can be placed in USER menu

broken line indicates a dynamic item, i.e. it is displayed only in particular selection/version

after pressing the key the set value will not be stored

after pressing the key the set value will be stored

30 continues on page 30

#### Setting the decimal point and the minus sign

##### DECIMAL POINT

Its selection in the menu, upon modification of the number to be adjusted it is performed by the control key with transition beyond the highest decade, when the decimal point starts flashing. Positioning is performed by /.

##### THE MINUS SIGN

Setting the minus sign is performed by the key on higher decade. When editing the item subtraction must be made from the current number (e.g.: 013 > , on class 100 > -87)

**Control keys functions**

Key	Measurement	Menu	Setting numbers/selection
	access into USER menu	exit menu	quit editing
	programmable key function	back to previous level	move to higher decade
	programmable key function	move to previous item	move down
	programmable key function	move to next item	move up
	programmable key function	confirm selection	confirm setting/selection
			numeric value is set to zero
	access into LIGHT/PROFI menu		
	direct access into PROFI menu		
		configuration of an item for "USER" menu	
		determine the sequence of items in "USER - LIGHT" menu	

**Setting items into „USER“ menu**

- in **LIGHT** or **PROFI** menu
- no items permitted in **USER** menu from manufacture
- on items marked by inverted triangle



**NO** item will not be displayed in USER menu

**YES** item will be displayed in USER menu with the option of setting

**SHOW** item will be solely displayed in USER menu

5.0

**Setting "LIGHT"****LIGHT****Simple programming menu**

- contains only items necessary for instrument setting and is protected by optional number code



- For capable users
- Only items necessary for instrument setting
- Access is password protected
- Possibility to arrange items of the „User“ menu
- Linear menu structure

**Preset from manufacture**

Password	"0"
Menu	LIGHT
USER menu	off
Setting the items	<b>DEF</b>

142.8

C + S

PASSW.

Access password

!

Upon delay exceeding 60 s the programming mode is automatically discontinued and the instrument itself restores the measuring mode

Selecting input and range

INPUTS

INP. I

TYPE I

E

MODE I

60 mV

RTD OHM

Selecting projection and connection

COHE I

2-WIRE

FORM.R

000.0

T/C

COHE I

EXT. ITC

GU.TEM

23

FORM.R

0000

DC PM OHM DU

MIN R

0

MAX R

100

FORM.R

0000

Option - comparator

LIML1

10

LIML2

20

LIML3

30

LIML4

40

LIML5

60

LIML6

70

LIML7

80

LIML8

90

Option - Analog output

TYPE.R.D.

I 20

MIN R.D.

0

MAX R.D.

100

Menu type

MENU

LIGHT

Return to manufacture calibration

CALIB

YES

Return to manufacture setting

SETTING

TYPE

DU

C.MIN

YES

C.MAX

YES

Calibration - only for "DU"

Language selection

L.RNG.

ENGL.

New password

N.PASS

0

Identification

ID.ENT.

YES

OMU 408...

142.8

Return to measuring mode

142.8



PAS5H



0

Entering access password  
for access into the menu

**PAS = 0**

- access into menu is unrestricted, after releasing keys you automatically move to first item of the menu

**PAS > 0**

- access into menu is protected by number code

**Set "Password" = 42**

Example

INPUT5



INP. 1

INP. 2

INP. 3

INP. 4

INP. 5

INP. 6

INP. 7

INP. 8



**INPUTS** Selection of the number of inputs

**Vstup 1** Example

- selection of input for its further setting
- inputs 5...8 get displayed only in the 8-channel version



### TYPE 1 Selection of the type of instrument

- primary selection of the type of instrument
- performs default setting **DEF** of values from manufacture, incl. calibration

TYPE 1	Menu	Type of instrument
DC	DC voltmeter	
PM	Process monitor	
OHM	Ohmmeter	
RTD-Pt	Thermometer for sensors Pt	
RTD-Ni	Thermometer for sensors Ni	
TC	Thermometer for thermocouples	
DU	Display for lin. potentiometer	
RTD-Cu	Thermometer for sensors Cu	

Type "PM"

TC      PM      TU      RT<sub>t</sub>-E

Example

Type "DC"	16
Type "PM"	18
Type "DU"	20
Type "OHM"	22
Type "RTD-Pt"	24
Type "RTD-Cu"	26
Type "RTD-Ni"	28
Type "T/C"	30

## Input/Channel A

DC

DC

DC

DC



DC

DC

DC

DC

DC

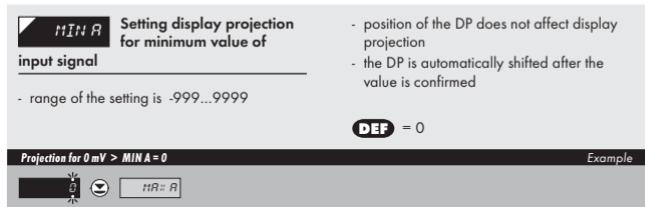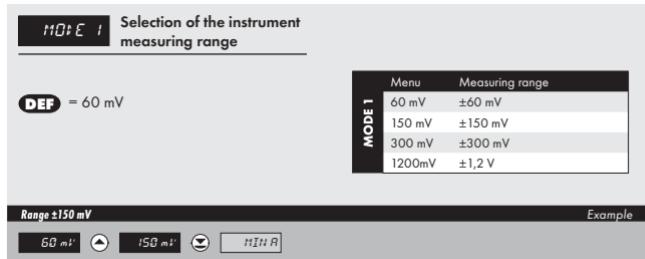

- position of the DP does not affect display projection
- the DP is automatically shifted after the value is confirmed



**MRxx.R** Setting display projection  
for maximum value of  
input signal


- range of the setting is -999...9999

- position of the DP does not affect display projection
- the DP is automatically shifted after the value is confirmed

**DEF** = 100

**Projection for 150 mV > MAX A = 3500**

Example									
100	100	100	200	200	200	300	300	300	400
500	0500	500	2500	2500	2500	3500	3500	3500	400

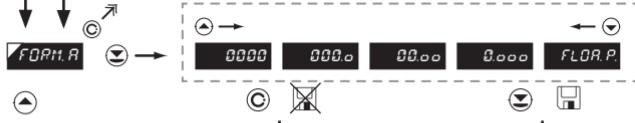

**FORMxx.R** Setting projection of the  
decimal point

**DEF** = 0000

- positioning of the DP is set here in the measuring mode

**Projection of DP on display > 0000**

0000	0000	0000	0000	0000	0000	0000	0000	0000	0000
0000	0000	0000	0000	0000	0000	0000	0000	0000	0000

\* subsequent item on the menu depends on instrument equipment

Type "PM"

**MODE 1 Selection of the instrument measuring range**

**DEF** = 4 - 20 mA

**Range 0...20 mA**

**MIN R Setting for minimum input signal**

**Projection for 0 mA > MIN A = -25**

**Example**

**Example**

**Menu Range**

Menu	Range
0-5mA	0...5 mA
0-20mA	0...20 mA
4-20mA	4...20 mA
0-2 V	$\pm 2$ V
0-5 V	$\pm 5$ V
0-10 V	$\pm 10$ V
0-40 V	$\pm 40$ V

- position of the DP does not affect display projection  
- the DP is automatically shifted after the value is confirmed

**DEF** = 0




**MAX.R** Setting display projection for maximum value of input signal

- range of the setting is -999...9999

- position of the DP does not affect display projection
- the DP is automatically shifted after the value is confirmed

**DEF = 100**

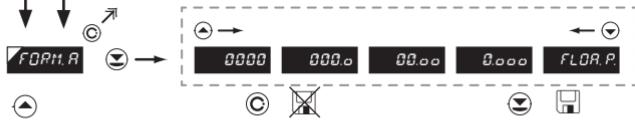


**FORM.R** Setting projection of the decimal point

**DEF = 0000**

- positioning of the DP is set here in the measuring mode



Type "DU"

Setting for minimum  
input signal

**MIN R** Setting display projection  
for minimum value of  
input signal

- range of the setting is -999...9999

- position of the DP does not affect display projection

- the DP is automatically shifted after the value is confirmed

**DEF** = 0

Example

Projection for the beginning &gt; MIN A = 0

Setting for maximum  
input signal

**MR% R** Setting display projection  
for maximum value of  
input signal

- range of the setting is -999...9999

- position of the DP does not affect display projection


- the DP is automatically shifted after the value is confirmed





**DEF** = 100

Example


Projection for the end &gt; MAX A = 5000



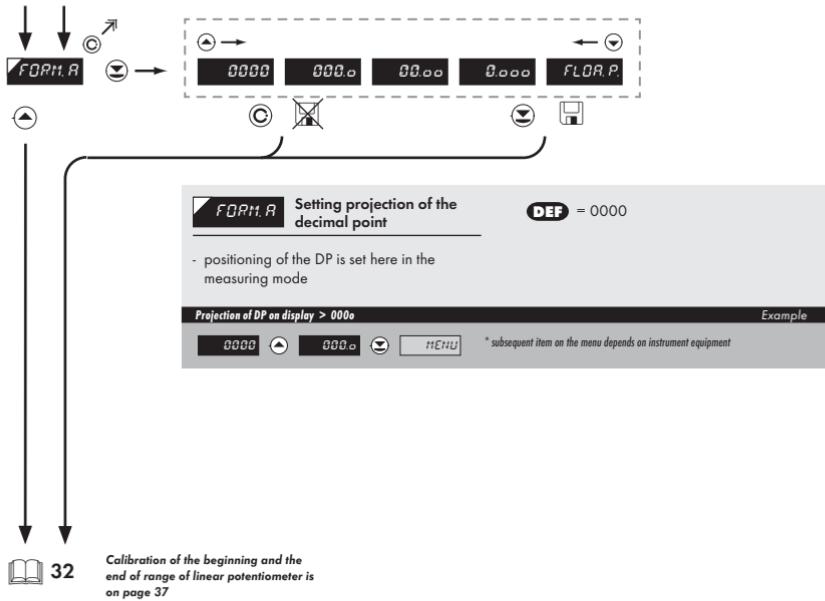

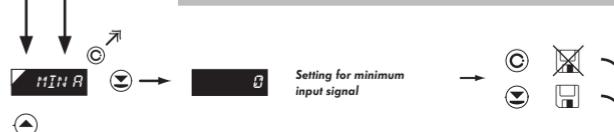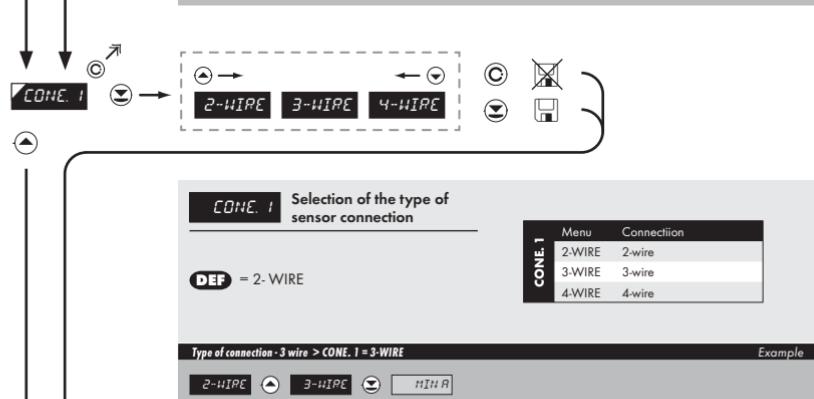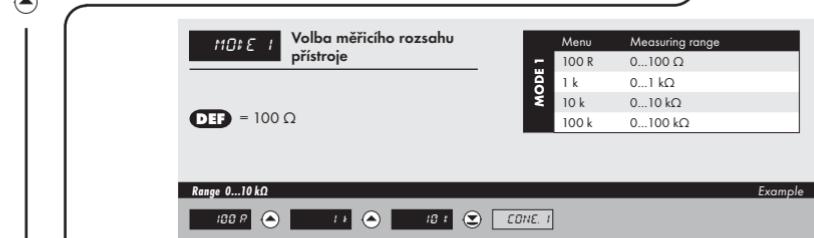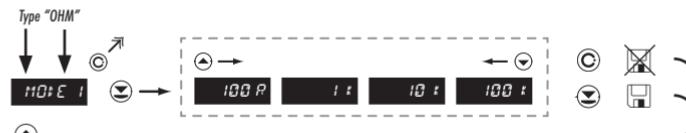


- position of the DP does not affect display projection
- the DP is automatically shifted after the value is confirmed

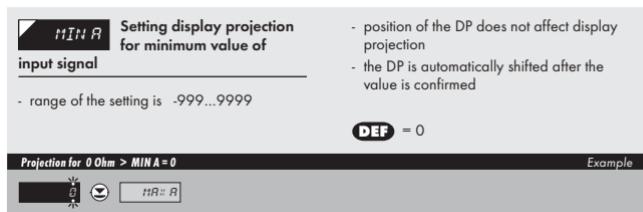



- position of the DP does not affect display projection
- the DP is automatically shifted after the value is confirmed

**DEF** = 100

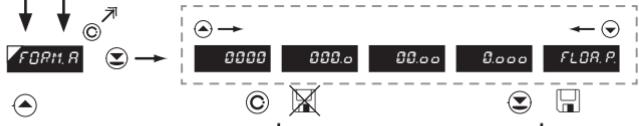


**DEF** = 0000

- positioning of the DP is set here in the measuring mode



\* subsequent item on the menu depends on instrument equipment

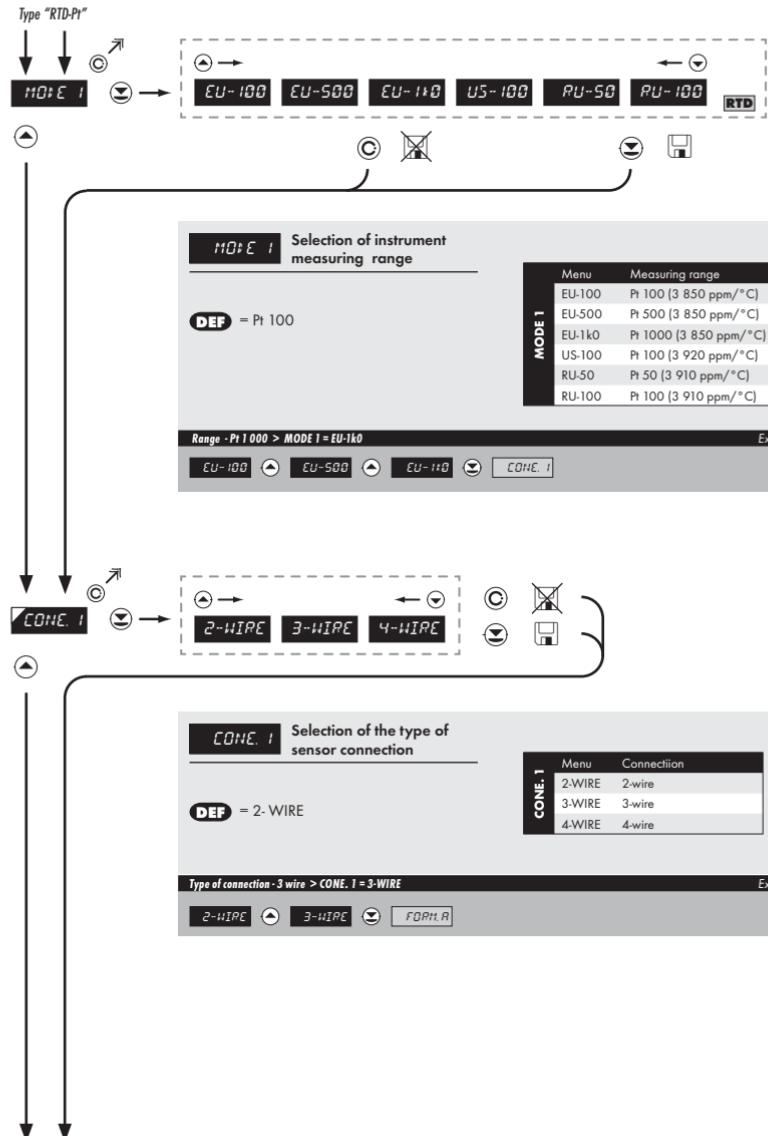




**FORM.R** Setting projection of the decimal point **DEF** = 0000

- positioning of the DP is set here in the measuring mode

**Projection of DP on display > 000a** Example

0000 000. \* subsequent item on the menu depends on instrument equipment

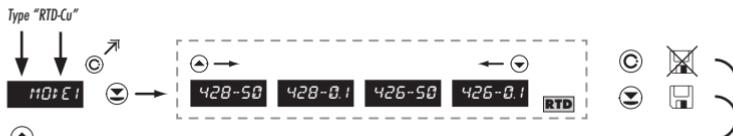

**MODE I** Selection of instrument measuring range

**DEF** = 428-50

Menu	Measuring range
428-50	Cu 50 (4 285 ppm/°C)
428-100	Cu 100 (4 285 ppm/°C)
426-50	Cu 50 (4 260 ppm/°C)
426-100	Cu 100 (4 260 ppm/°C)

Range - Cu-50/4 260 ppm > MODE. I = 426-50

Example

428-50 428-0.1 426-50 **CONE. I**



**CONE. I** Selection of the type of sensor connection

**DEF** = 2-WIRE

Menu	Connection
2-WIRE	2-wire
3-WIRE	3-wire
4-WIRE	4-wire

Type of connection - 3 wire > CONE. I = 3-WIRE

Example

2-WIRE 3-WIRE **FORM.R**



**FORM.R** Setting projection of the decimal point DEF = 0000

- positioning of the DP is set here in the measuring mode

**Projection of DP on display > 000e** Example

0000 ⌂ 000.e ⌃ MENU \* subsequent item on the menu depends on instrument equipment



**MODE 1 Selection of instrument measuring range**

**DEF** = Ni 1 000 - 5 000 ppm/°C

**Rangr - Ni 10 000/5 000 ppm > MODE 1 = 5.0-10k**

5.0-1k    6.2-1k    5.0-10k    6.2-10k    **CONE. 1**

Example

Menu	Measuring range
5.0-1k	Ni 1 000 (5 000 ppm/°C)
6.2-1k	Ni 1 000 (6 180 ppm/°C)
5.0-10k	Ni 10 000 (5 000 ppm/°C)
6.2-10k	Ni 10 000 (6 180 ppm/°C)



**CONE. 1 Selection of the type of sensor connection**

**DEF** = 2-WIRE

**Type of connection - 3-wire > CONE. 1 = 3-WIRE**

2-WIRE    3-WIRE    **FORM1 R**

Example

Menu	Connection
2-WIRE	2-wire
3-WIRE	3-wire
4-WIRE	4-wire



**FORM.R** Setting projection of the decimal point **DEF** = 0000

- positioning of the DP is set here in the measuring mode

**Projection of DP on display > 000a** Example

0000 000. \* subsequent item on the menu depends on instrument equipment

Type "T/C"



( $\circlearrowleft$ )  $\rightarrow$   
 T/C B T/C E T/C J T/C K  
 > T/C N T/C R T/C S T/C T T/C F ( $\circlearrowleft$ )



### MODE 1 Selection of the type of thermocouple

- setting the input range depends on the measuring range ordered

**DEF** = Type "J"

Menu	Type of thermocouple
T/C B	B
T/C E	E
T/C J	J
T/C K	K
T/C N	N
T/C R	R
T/C S	S
T/C T	T

Example

Type of thermocouple "K"



( $\circlearrowleft$ )  $\rightarrow$   
 INT.1TC INT.2TC EXT.1TC EXT.2TC ( $\circlearrowleft$ )



### CONE. 1 Selection of the type of sensor connection

**DEF** = EXT. 1TC

Menu	Connection	Ref. T/C
INT.1TC	measuring C.J. at instrument brackets	x
INT.2TC	measuring C.J. at instrument brackets with anti-series connected ref. TC	✓
EXT.1TC	the entire measuring set is working under inviaried and constant temperature	x
EXT.2TC	when using compensation box	✓

Example

Type of connection &gt; CONE. 1 = EXT. 2TC



**C.J. TEM** Setting temperature of cold junction

- range 0...99 °C with compensation box


- položka je přístupná pouze při nastavení parametrů 1. vstupu

**DEF** = 23

## Setting temperature of cold junction &gt; C.J. TEM. = 35

Example

23 ⌂ 24 ⌂ 25 ⌂ 26 ⌂ 27 ⌂ 28 ⌂ FORM.R

**FORM.R** Setting projection of the decimal point**DEF** = 0000

- positioning of the DP is set here in the measuring mode

## Projection of DP on display &gt; 0000

Example

0000 ⌂ 000.0 ⌂ MENU

\* subsequent item on the menu depends on instrument equipment

!

For thermocouple type "B" the items CONE. 1 and C.J. TEM. are not available

!


Method and procedure of setting the cold junctions is described in separate chapter on page 76

Displayed only with options > Comparators




- contingent modification of hysteresis or delay may be performed in "PROFI" menu

- range of the setting is -99999...999999
- default "Hysteresis"=0 "Delay"=0



- contingent modification of hysteresis or delay may be performed in "PROFI" menu

- range of the setting is -99999...999999
- default "Hysteresis"=0 "Delay"=0

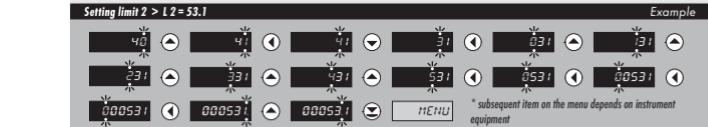

Items for "Limits" and "Analog output" are accessible only if incorporated in the instrument.



**LIM L3** Setting boundary for limit 3

- contingent modification of hysteresis or delay may be performed in "PROFI" menu
- range of the setting is -99999...999999
- default "Hysteresis"=0 "Delay"=0

**DEF** = 60

Setting limit 3 > L3 = 85

60 61 62 63 64 65 66 67 68 69

65 66 67 68 69 MENU

Example

\* subsequent item on the menu depends on instrument equipment



**LIM L4** Setting boundary for limit 4

- contingent modification of hysteresis or delay may be performed in "PROFI" menu
- range of the setting is -99999...999999
- default "Hysteresis"=0 "Delay"=0

**DEF** = 80

Setting limit 4 > L4 = 103

80 81 82 83 84 85 86 87 88 89

83 84 85 86 87 88 89 MENU

Example

\* subsequent item on the menu depends on instrument equipment

!

If instrument with 8 relays was ordered, after setting Limit 4 follows the setting of limits 5...8.

Displayed only with options > **Analog output**

**TYP.R.O.** Setting the type of analog output

Menu	Range	Description
0-20mA	0...20 mA	
E-4-20mA	4...20 mA	with indication of error statement [ $<3,6$ mA]
4-20mA	4...20 mA	
0-5mA	0...5 mA	
0-2 V	0...2 V	
0-5 V	0...5 V	
0-10 V	0...10 V	

**DEF** = 4...20 mA

Type of analog output-0...10 V > TYP. A.O. = 0-10 V      Example

**MIN.R.O.** Assigning the display value to the beginning of the AO range


**DEF** = 0

- range of the setting is -999...9999

Display value for the beginning of the AO range > MIN.A.O. = 0      Example

**MIN.R.O.** !

Items for "Limits" and "Analog output" are accessible only if incorporated in the instrument.

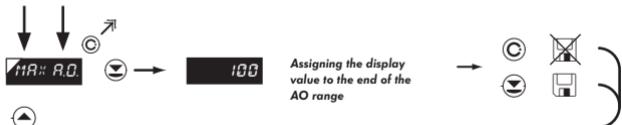


**Max A.O.** Assigning the display value to the end of the AO range      DEF = 100

- range of the setting is -999...9999

Display value for the end of the AO range > MAX A.O. = 120      Example

100 100 10 120 MENU

Displayed only with options > **Analog output**

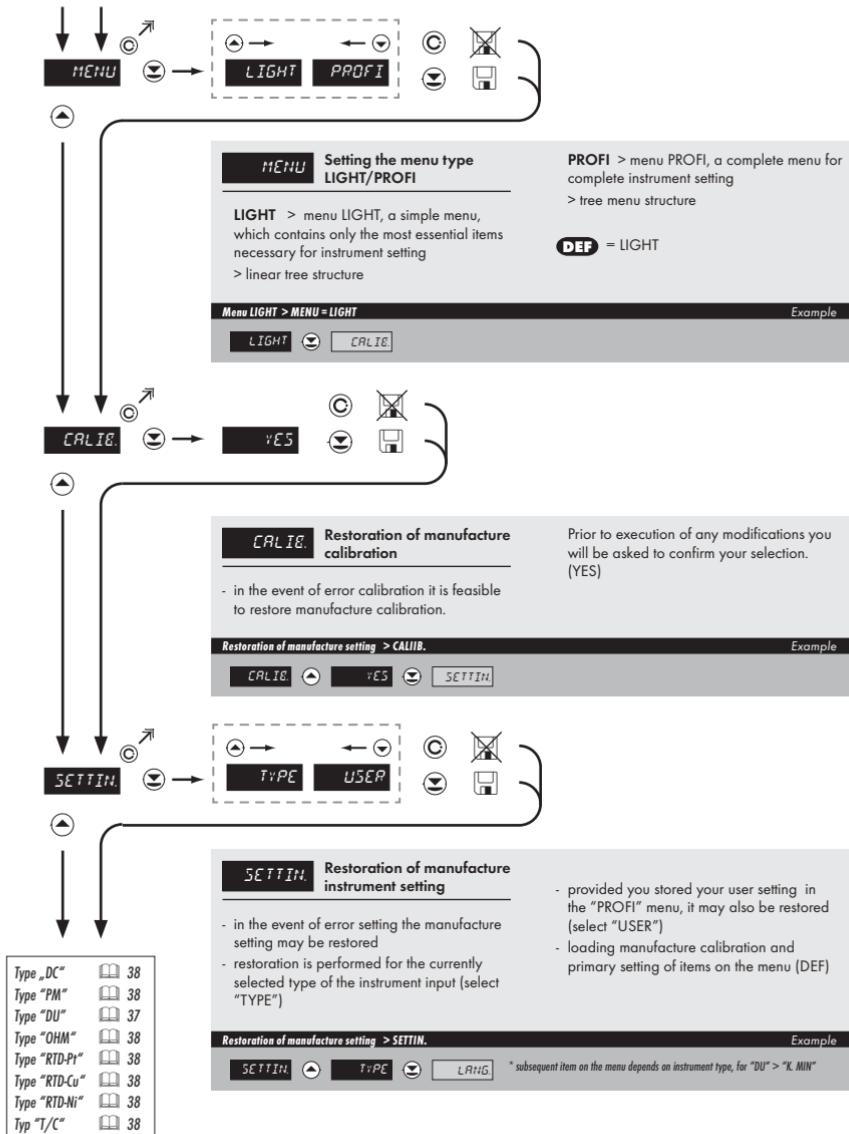

Type "DU"



**C.MIN** Calibration of input range -  
the potentiometer traveller  
in initial position

Only for type "DU"

- the inputs for calibration always include only active inputs, i.e. those that are set for "MOD > DU".

## Calibration of the beginning of the range &gt; C.MIN

Example

YES C.MIN



**C.MAX** Calibration of input range -  
the potentiometer traveller  
in end position

Only for type "DU"


- the inputs for calibration always include only active inputs, i.e. those that are set for "MOD > DU".

## Calibration of the end of the range &gt; C.MAX

Example

YES LARG

- prior confirming the flashing "YES" sign the potentiometer traveller has to be in given idle position

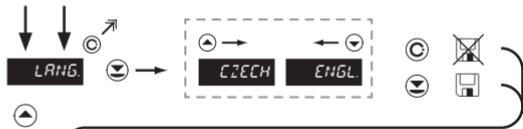

**LANG.** Selection of language in instrument menu

- selection of language version of the instrument menu **DEF** = ENGL

**Language selection - ENGLISH > LANG. = ENGL.** Example

CZECH ENGL N.PASS




**N.PASS.** Setting new access password

- access password for menu LIGHT/PROFI  
- range of the number code 0...9999

**DEF** = 0

**New password - 341 > N.PASSW. = 341** Example

01 02 03 04 05 06 07 08 09 00  
41 81 11 21 31 71 91 51 61 01  
41 81 11 21 31 71 91 51 61 31

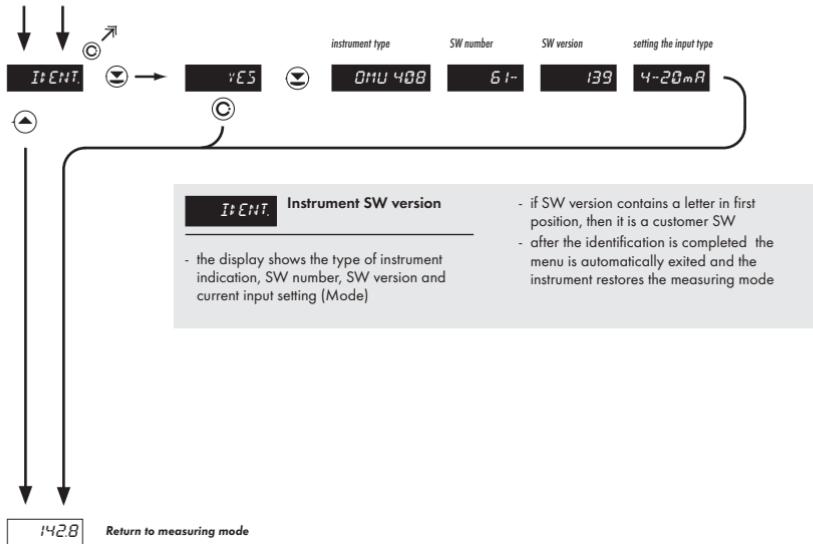

6.0

**Setting "PROFI"****PROFI****Complete programming menu**

- contains complete instrument menu and is protected by optional number code
- designed for expert users
- preset from manufacture is menu **LIGHT**

SETTING PROFI



- For expert users
- Complete instrument menu
- Access is password protected
- Possibility to arrange items of the „User“ menu
- Tree menu structure

**Switching over to "PROFI" menu**


- temporary switch-over to **PROFI** menu, which is suitable to edit a few items
- after quitting **PROFI** menu the instrument automatically switches to **LIGHT** menu
- access is password protected (if it was not set under item N. PASS. =0)



- access into **LIGHT** menu and transition to item „MENU“ with subsequent selection of „PROFI“ and confirmation
- after re-entering the menu the **PROFI** type is active
- access is password protected (if it was not set under item N. PASS. =0)




## 6.1 Setting "PROFI" - INPUT



The primary instrument parameters are set in this menu

- |                 |   |
|-----------------|---|
| <b>CLEAR</b>    | Resetting internal values                             |
| <b>CONFIG.</b>  | Selection of measuring range and parameters           |
| <b>RTC</b>      | Setting date and time for option with RTC             |
| <b>EXT. IN.</b> | Setting external inputs functions                     |
| <b>fEV5</b>     | Assigning further functions to keys on the instrument |

## 6.1.1 Resetting internal values

**CLEAR** Resetting internal values

- |                |                         |
|----------------|-------------------------|
| <b>CL.TAR.</b> | Tare resetting          |
| <b>CL.MM</b>   | Resetting min/max value |

- resetting memory for the storage of minimum and maximum value achieved during measurement

- |               |                                 |
|---------------|---------------------------------|
| <b>CL.MEM</b> | Resetting the instrument memory |
|---------------|---------------------------------|
- resetting memory with data measured in the "FAST" or "RTC" modes  
 - not in standard equipment

## 6.1.2a Selection of measuring rate

↑    ← →    ↓

INPUTS	CLEAR	PERIOD'S	40.0
CHANNEL	CONFIG	INPUTS	20.0
OUTPUT	RTC	IN.MOD.	10.0
SERVICE	EXT.IN	SWITCH	5.0
	IEV'S	TIM.PR.	2.0
		INP. 1	1.0
		INP. 2	0.5
		INP. 3	0.2
		INP. 4	0.1
		INP. 5	
		INP. 6	
		INP. 7	
		INP. 8	

DEF

## PERIOD'S Selection of measuring rate

40.0	40,0 measurements/s
20.0	20,0 measurements/s
10.0	10,0 measurements/s
5.0	5,0 measurements/s
2.0	2,0 measurements/s
1.0	1,0 measurements/s
0.5	0,5 measurements/s
0.2	0,2 measurements/s
0.1	0,1 measurements/s

## 6.1.2b Selection of number of active measuring inputs

↑    ← →    ↓


INPUTS	CLEAR	PERIOD'S	1 INP.
CHANNEL	CONFIG	INPUTS	2 INP.
OUTPUT	RTC	IN.MOD.	3 INP.
SERVICE	EXT.IN	SWITCH	4 INP.
	IEV'S	TIM.PR.	5 INP.
		INP. 1	6 INP.
		INP. 2	7 INP.
		INP. 3	8 INP.
		INP. 4	
		INP. 5	
		INP. 6	
		INP. 7	
		INP. 8	

DEF

## INPUTS Selection of number of active inputs

- the number of active measuring inputs influences the resulting measuring rate		
	1 active measuring input	
	2 INP.	2 active measuring inputs
	3 INP.	3 active measuring inputs
	4 INP.	4 active measuring inputs
	5 INP.	5 active measuring inputs
	6 INP.	6 active measuring inputs
	7 INP.	7 active measuring inputs
	8 INP.	8 active measuring inputs

## 6.1.2c Selection of measuring mode

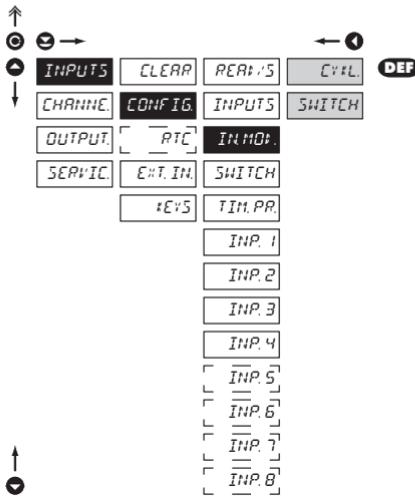**IN.MOT.** Selection of measuring mode


**CYCL.** Cyclic measurement on all inputs

- number of active measuring inputs is set in the menu INPUTS/CONFIG/OUTPUTS
- projection of measuring inputs is set in the menu INPUTS/CONFIG/SWITCHIN.
- the cycle option rather significantly affects the measuring rate and depends on the number of active inputs (real measuring rates are listed in chapter Technical data)

**SWITCH** Instrument performs measuring only on the active input

- projection of measuring inputs is set in the menu INPUTS/CONFIG/SWITCH.

## 6.1.2d Selection of measuring inputs switching

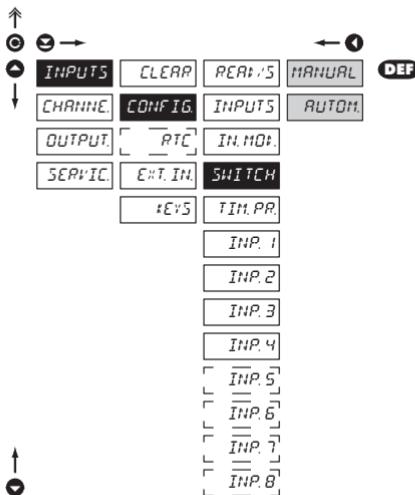**IN.MOT.** Selection of measuring inputs switching


**MANUAL** Manual inputs switching

- inputs switching is controlled by selected key on the front panel or selected external input

**AUTOM.** Automatic inputs switching


- inputs switching is automatic with time period set in "TIM.SW."

## 6.1.2e Setting period for measuring inputs switching

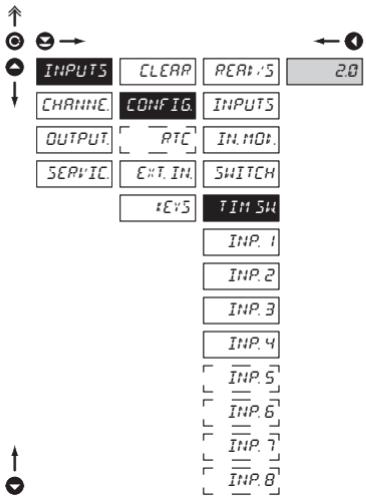**TIM 5H.** Setting period for inputs switching

- setting time period for projection of channels in automatic mode of inputs switching ("AUTOM.")
- range of setting 0,5...99,9 s
- **DEF** = 2 s

## 6.1.2f Selection of „instrument” type for Input 1

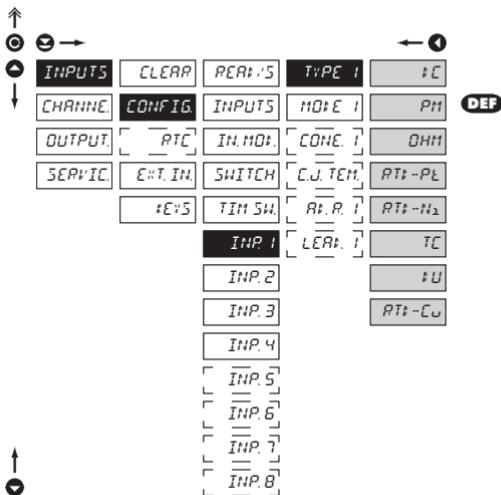**TYPE 1** Selection of „instrument” type for Input 1

- selection of particular type of "instrument" is bound to relevant dynamic items

TC	DC voltmeter
PH	Process monitor
OHM	Ohmmeter
RTt-Pt	Thermometer for Pt xxx
RTt-N <sub>1</sub>	Thermometer for Ni xxxx
TC	Thermometer pro thermocouples
TU	Display for linear potentiometers
RTt-Cu	Thermometer for Cu xxx

## 6.1.2g Selection of measuring range for Input 1

↑    →    ←    ↓



<b>INPUTS</b>	<b>CLEAR</b>	<b>REF/VS</b>	<b>TYPE I</b>	<b>60mV</b>	<b>100 R</b>	<b>OHM</b> ← → <b>DEF</b>
<b>CHANNEL</b>	<b>CONFIG.</b>	<b>INPUTS</b>	<b>MODE I</b>	<b>150mV</b>	<b>1 k</b>	
<b>OUTPUT</b>	<b>RTC</b>	<b>IN.MOT</b>	<b>CONF. I</b>	<b>300mV</b>	<b>10 k</b>	
<b>SERVIC.</b>	<b>EXT. IN.</b>	<b>SWITCH</b>	<b>C.J. TEMP.</b>	<b>1200mV</b>	<b>100 k</b>	
			<b>FEV5</b>	<b>TIM SH.</b>	<b>RT. R. I</b>	
			<b>INP. I</b>			<b>LERT. I</b>
			<b>INP. 2</b>	<b>0-5mA</b>	<b>PM</b>	
			<b>INP. 3</b>	<b>0-20mA</b>		
			<b>INP. 4</b>	<b>4-20mA</b>		
			<b>INP. 5</b>	<b>0-2 V</b>		
			<b>INP. 6</b>	<b>0-5 V</b>		
			<b>INP. 7</b>	<b>0-10 V</b>		
			<b>INP. 8</b>	<b>0-40 V</b>		
			<b>DEF</b>			
			<b>RTD-Pt</b>			<b>RTD-Cu</b>
			<b>EU-100</b>	<b>428-S0</b>	<b>DEF</b>	
			<b>EU-500</b>	<b>428-0.1</b>		
			<b>EU-1k0</b>	<b>426-S0</b>		
			<b>US-100</b>	<b>426-0.1</b>		
			<b>RU-50</b>			
			<b>RU-100</b>			
			<b>DEF</b>			
			<b>RTD-Ni</b>			<b>T/C</b>
			<b>5.0-1k</b>	<b>T/C E</b>		
			<b>5.2-1k</b>	<b>T/C J</b>		
			<b>5.0-10k</b>	<b>T/C N</b>		
			<b>5.2-10k</b>	<b>T/C R</b>		
			<b>DEF</b>			
			<b>DU</b>			<b>T/C S</b>
			<b>LIN.POT.</b>	<b>T/C T</b>		
			<b>DEF</b>			<b>T/C L</b>

Mode I Selection of instrument measuring range - INP 1	
DC	Menu Measuring range
	60 mV ±60 mV
	150 mV ±150 mV
	300 mV ±300 mV
	1200 mV ±1,2 V
PM	Menu Measuring range
	0-5 mA 0...5 mA
	0-20 mA 0...20 mA
	4-20 mA 4...20 mA
	0-2 V ±2 V
	0-5 V ±5 V
	0-10 V ±10 V
	0-40 V ±40 V
OHM	Menu Measuring range
	100 R 0...100 Ω
	1 k 0...1 kΩ
	10 k 0...10 kΩ
	100 k 0...100 kΩ
	AUTO Automatická změna rozsahu
RTD-Pt	Menu Measuring range
	EU-100 Pt 100 (3 850 ppm/°C)
	EU-500 Pt 500 (3 850 ppm/°C)
	EU-1k0 Pt 1000 (3 850 ppm/°C)
	US-100 Pt 100 (3 920 ppm/°C)
	RU-50 Pt 50 (3 910 ppm/°C)
	RU-100 Pt 100 (3 910 ppm/°C)
RTD-Ni	Menu Measuring range
	5.0-1k Ni 1 000 (5 000 ppm/°C)
	6.2-1k Ni 1 000 (6 180 ppm/°C)
	5.0-10k Ni 10 000 (5 000 ppm/°C)
	6.2-10k Ni 10 000 (6 180 ppm/°C)
RTD-Cu	Menu Measuring range
	428-50 Cu 50 (4 280 ppm/°C)
	428-0.1 Cu 1 00 (4 280 ppm/°C)
	426-50 Cu 50 (4 260 ppm/°C)
	426-0.1 Cu 100 (4 260 ppm/°C)
T/C	Menu Type of thermocouple
	T/C B B
	T/C E E
	T/C J J
	T/C K K
	T/C N N
	T/C R R
	T/C S S
	T/C T T
	T/C L L

\* Setting procedure is identical also for inputs 2...8

## 6.1.2h Selection of type of sensor connection

RTD OHM T/C

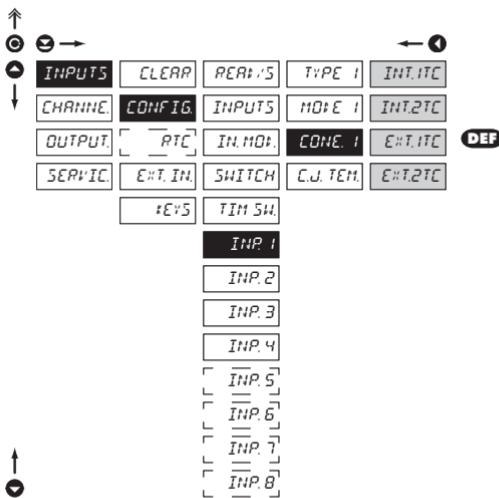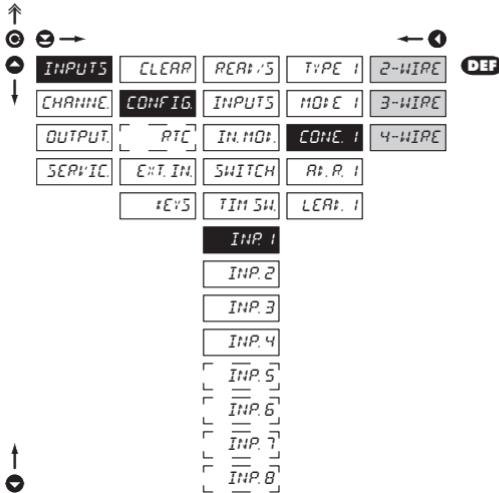

## CONE. I Selection of type of sensor connection

RTD OHM

2-wire connection

3-wire connection

4-wire connection

T/C

## INT.ITE Measurement without reference thermocouple

- measuring cold junction at instrument brackets

## INT.2TC Measurement with reference thermocouple

- measuring cold junction at instrument brackets with anti-series connected reference thermocouple

## EXT.ITE Measurement without reference thermocouple

- the entire measuring set is working under invaried and constant temperature

## EXT.2TC Measurement with reference thermocouple

- when using compensation box



Setting for "T/C" is accessible only for 1st input




Method and procedure of setting the cold junctions is described in separate chapter on page 84




For thermocouple type "B" the items CONE. and C.J. TEM. are not available



Setting procedure is identical also for inputs 2...8

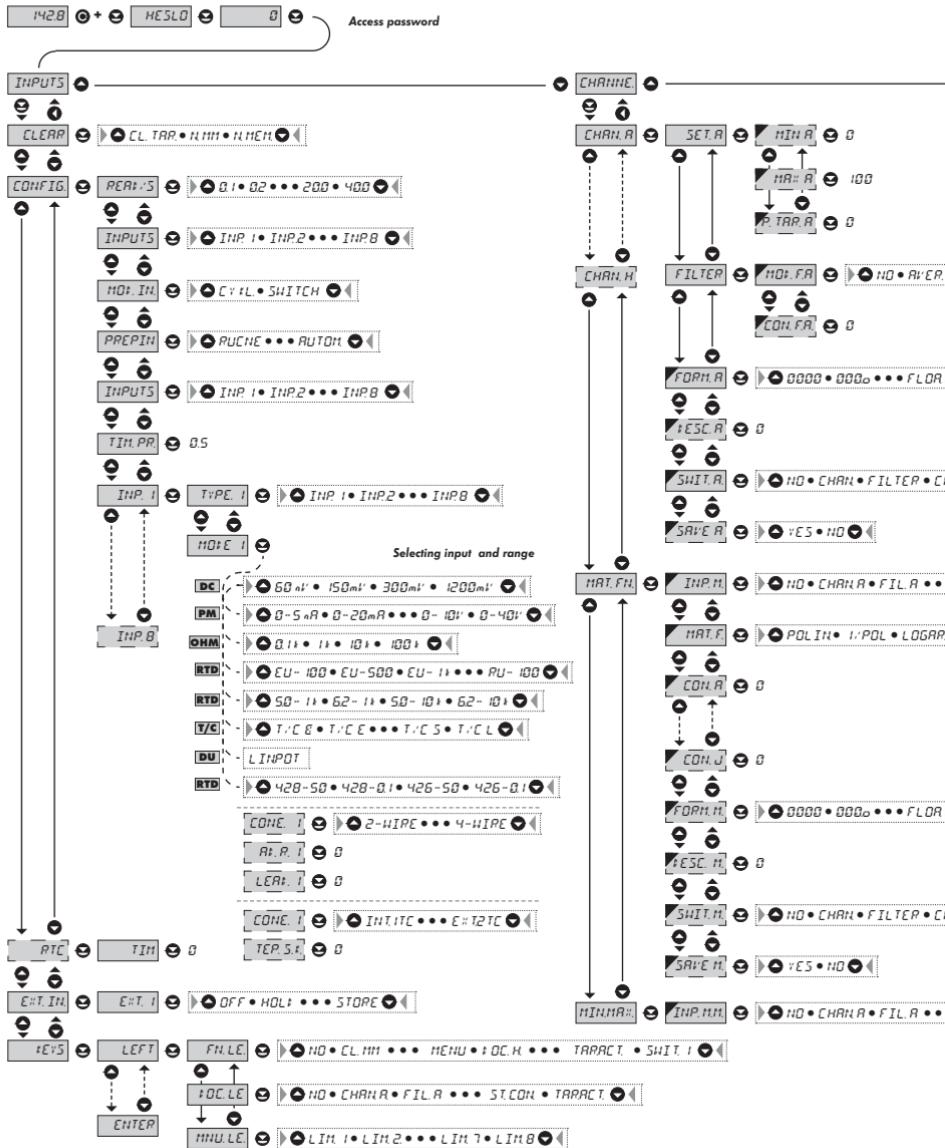

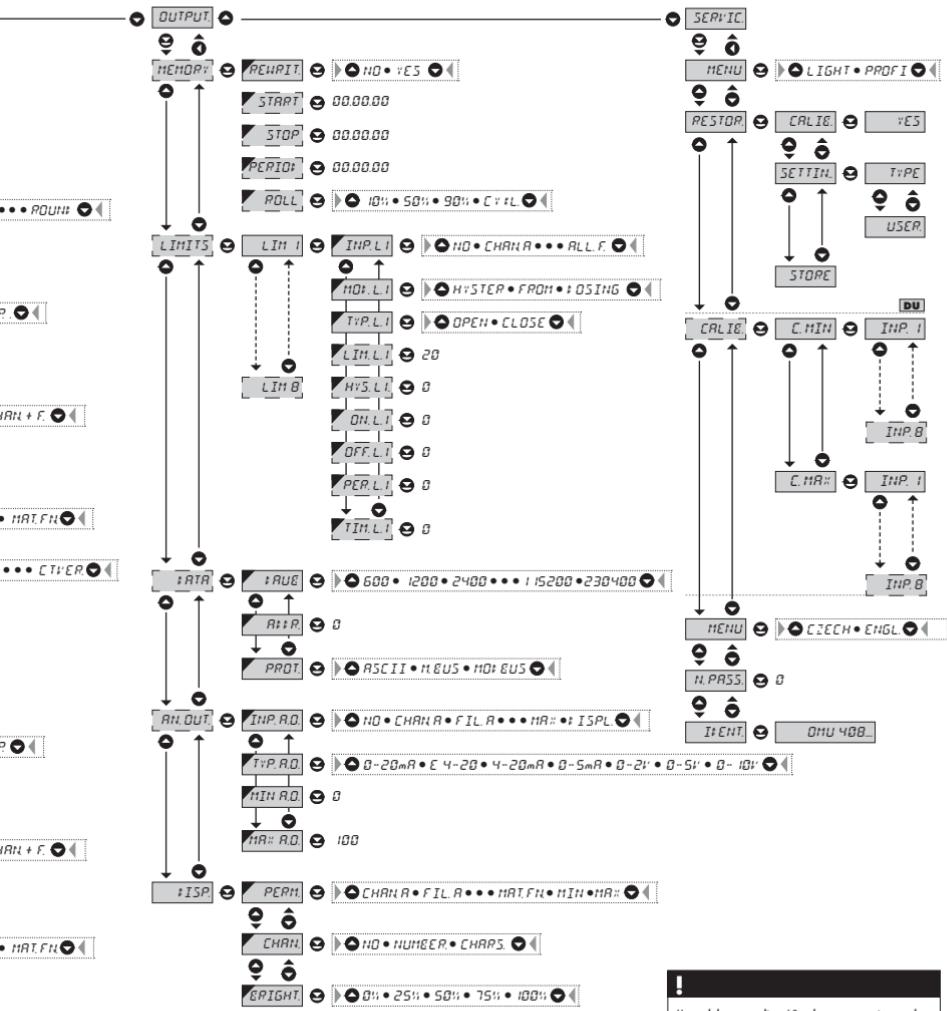

## 6.1.2i Setting temperature of cold junction

**INPUTS** **CLEAR** **PERIOD** **TYPE** I **23**

**CHANNEL** **CONFIG** **INPUTS** **MODE** I

**OUTPUT** **RTC** **IN.MOT** **CONE** I

**SERVIC.** **EXT. IN** **SWITCH** **C.J. TEM.**

**#EV5** **TIM SH.**

**INP. 1**  
**INP. 2**  
**INP. 3**  
**INP. 4**  
**INP. 5**  
**INP. 6**  
**INP. 7**  
**INP. 8**

**C.J. TEM.** Setting temperature of cold junction

- range 0...99°C with compensation box

- **DEF** = 23°C



Setting for "T/C" is accessible only for 1st input

## 6.1.2j Compensation of 2-wire conduct

**RTD** **OHM**

**INPUTS** **CLEAR** **PERIOD** **TYPE** I **0**

**CHANNEL** **CONFIG** **INPUTS** **MODE** I

**OUTPUT** **RTC** **IN.MOT** **CONE** I

**SERVIC.** **EXT. IN** **SWITCH** **R<sub>B</sub>. R<sub>I</sub>**

**#EV5** **TIM SH.** **LEAF. I**

**INP. 1**  
**INP. 2**  
**INP. 3**  
**INP. 4**  
**INP. 5**  
**INP. 6**  
**INP. 7**  
**INP. 8**

**R<sub>B</sub>. R<sub>I</sub>** Offset of the beginning of the measuring range

- in cases when it is necessary to offset the beginning of the range by certain value, e.g. while using sensor in measuring head

- entered directly in Ohm (0...9999)


- **DEF** = 0



Setting procedure is identical also for inputs 2...8

## 6.1.2k Compensation of 2-wire conduct

RTD OHM

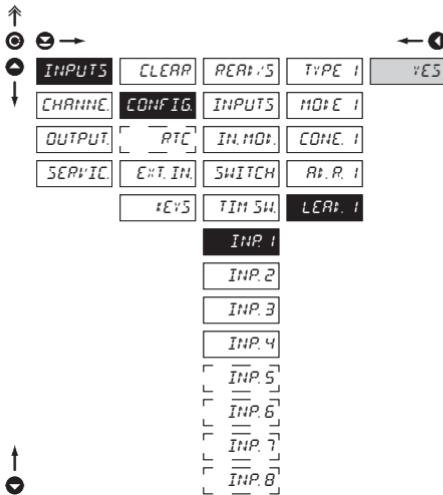


## LERT. I Compensation of 2-wire conduct

- for measurement accuracy it is necessary to perform compensation of conduct always in case of 2-wire connection
- prior confirmation of the displayed prompt „YES“ it is necessary to substitute the sensor at the end of the conduct by a short-circuit
- **DEF** = 0

\*

Setting procedure is identical also for inputs 2...8

## 6.1.3 Setting the real time clock



## RTC Setting the real time clock (RTC)

TIME Time setting

- format 23.59.59

RATE Date setting

- format DD.MM.YY

## 6.1.4a External input function selection


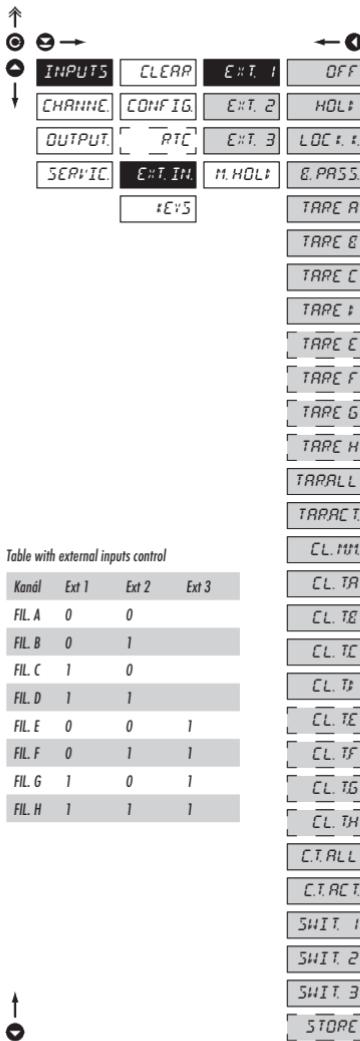


Table with external inputs control

Kanal	Ext 1	Ext 2	Ext 3
FIL A	0	0	
FIL B	0	1	
FIL C	1	0	
FIL D	1	1	
FIL E	0	0	1
FIL F	0	1	1
FIL G	1	0	1
FIL H	1	1	1

External input function selection	
<b>OFF</b>	Input is off
<b>HOLD</b>	Activation of HOLD
<b>LOCK</b>	Locking keys on the instrument
<b>E.PASS.</b>	Activation of locking access into programming menu LIGHT/PROFI
<b>TARE</b>	Tare activation > by individual inputs
<b>TARE ALL</b>	Tare activation on all channels
<b>TARE ACT.</b>	Tare activation on current input
<b>CL.MM.</b>	Resetting min/max value
<b>CL.T.-</b>	Clear tare > by individual inputs
<b>CL.T. ALL</b>	Clear tare on all channels
<b>CL.ACT.</b>	Clear tare on current input
<b>SHIT. 1</b>	Gradual switching of inputs projection
<b>SHIT. 2</b>	BCD switching of inputs projection - Ext 1, 2
- control see table	
- after this choice the setting for „EXT.2“ is automatically disabled	
<b>SHIT. 3</b>	BCD switching of inputs projection - Ext 1, 2
- control see table	
- after this choice the setting for „EXT.2“ and „EXT. 3“ is automatically disabled	
<b>STORE</b>	Activation of recording of measured data into instrument memory (not a standard option)
- <b>DEF</b>	EXT. 1 > HOLD
- <b>DEF</b>	EXT. 2 > LOCK
- <b>DEF</b>	EXT. 3 > SHIT. 1
*	
Setting procedure is identical for EXT. 2 and EXT. 3	


## 6.1.4b Selection of function "HOLD"

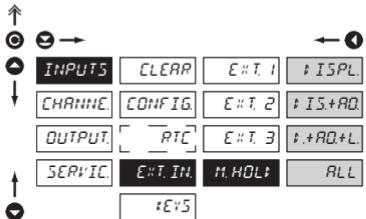

## M.HOLD Selection of function "HOLD"

- tISPL. "HOLD" locks only the value displayed
- tIS+AO. "HOLD" locks the value displayed and on AO
- tAO+L. "HOLD" locks the value displayed, on AO and limit evaluation
- ALL "HOLD" locks the entire instrument

## 6.1.5a Optional accessory functions of the keys

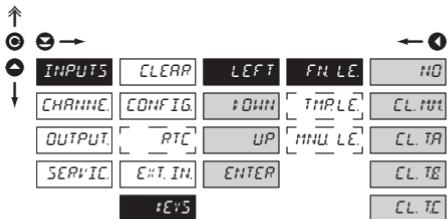


## FN. LE. Assigning further functions to instrument keys

- „FN. LE.“ > executive functions
- „TMP. LE.“ > temporary projection of selected values
- „MNU. LE.“ > direct access into menu on selected item
- NO** Key has no further function
- CL.MI** Resetting min/max value
- CL.TA** Clear tare > by individual inputs
- CL.TB** Clear tare on all channels
- CL.RET.** Clear tare on current input
- MENU** Direct access into menu on selected item
- after confirmation of this selection the „MNU. LE.“ item is displayed on superior menu level, where required selection is performed
- TEMP. K** Temporary projection of selected values
- after confirmation of this selection the item „TMP. LE.“ is displayed on superior menu level, where required selection is performed



<b>TARE -</b>	Tare activation > by individual inputs
<b>TARE ALL</b>	Tare activation on all channels
<b>TARE ACT.</b>	Tare aktivation on current input
<b>SHIT. I</b>	Gradual switching of inputs projection

#### 6.1.5b Optional accessory functions of the keys - Temporary projection

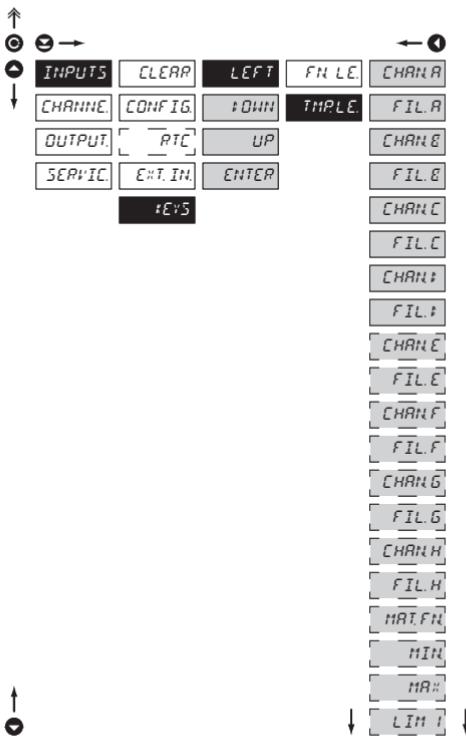

##### **TMPL.E** Temporary projection of selected item

- "Temporary" projection of selected value is displayed for the time of keystroke
- "Temporary" projection may be switched to permanent by pressing **◎ + Selected key**, this holds until the stroke of any key

##### **CHAN. -** Temporary projection of value input/channel

- selection from "Temporary" projection of input A, B, C, D, E, F, G, H

##### **FIL. -** Temporary projection of value input/channel after digital filter processing

- selection from "Temporary" projection of filtered input A, B, C, D, E, F, G, H

##### **MAT.FN.** Temporary projection of value "Mathematic funktion"

- **MIN** Temporary projection of value "Min. value"

##### **MR#** Temporary projection of value "Max. value"

- **LIM** Temporary projection of value "Limits"

- selection from "Temporary" projection Limits 1, 2, 3, 4, 5, 6, 7, 8



Setting is identical for LEFT, DOWN, UP and ENTER



- LIM -** Temporary projection of value "Limits"
  - selection from "Temporary" projection Limits 1, 2, 3, 4, 5, 6, 7, 8
- TIME** Temporary projection of "TIME" value
- RATE** Temporary projection of "DATE" value
- TARE -** Temporary projection of "TARE" value
  - selection from "Temporary" projection Tare for input A, B, C, D, E, F, G, H
- TARE.FT** Temporary projection of value "TARE"
  - "Temporary" projection of Tare for currently selected type
- P.TAR.A** Temporary projection of value "P. TAR. A"
  - selection from "Temporary" projection of "Fixed tare" for inp. A, B, C, D, E, F, G, H
- P.T.R.FT** Temporary projection of value "P. T. ACT."
  - "Temporary" projection of "Fixed tare" for currently selected input
- ST.CON** Temporary projection of "CJC" value




Setting is identical for LEFT, DOWN, UP and ENTER



Preset values of the control keys **DEF**:

LEFT	Show Tare
UP	Show Max. value
DOWN	Show Min. value
ENTER	w/o functione

## 6.1.5c Optional accessory functions of the keys - Direct access to item

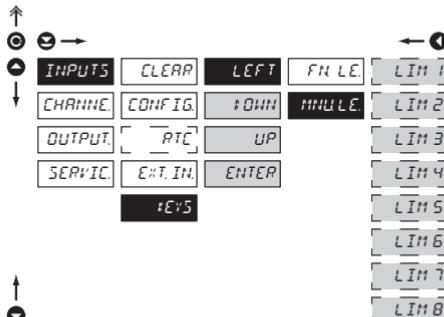

## MNULE

Assigning access to selected menu item


- LIM 1 Direct access to item "LIM 1"
- LIM 2 Direct access to item "LIM 2"
- LIM 3 Direct access to item "LIM 3"
- LIM 4 Direct access to item "LIM 4"
- LIM 5 Direct access to item "LIM 5"
- LIM 6 Direct access to item "LIM 6"
- LIM 7 Direct access to item "LIM 7"
- LIM 8 Direct access to item "LIM 8"



Setting is identical for LEFT, DOWN, UP and ENTER



## 6.2 Setting "PROFI" - CHANNELS

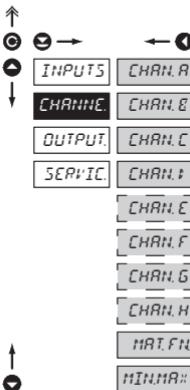

The primary instrument parameters are set in this menu

**CHAN.R** Setting parameters of measuring "Channel"


- selection from inputs A, B, C, D, E, F, G, H

**MATH.FN** Setting parameters of mathematic functions

**MIN.MAX** Selection of access and evaluation of Min/max value

## 6.2.1a Display projection

DC PM DU OHM

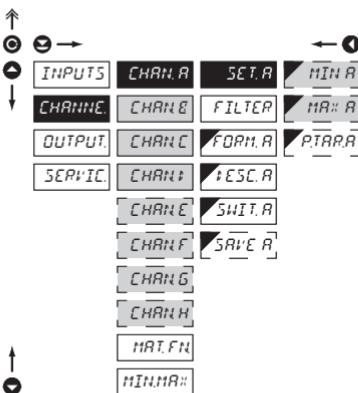

**SET.R** Setting display projection - Input A

**MIN.R** Setting display projection for minimum value of input signal

- range of the setting is -999...9999

- **DEF** = 0

**MAX.R** Setting display projection for maximum value of input signal

- range of the setting is -999...9999


- **DEF** = 100



Setting is identical for input B, C, D, E, F, G, H

## 6.2.1b Setting fixed tare

DC PM DU OHM

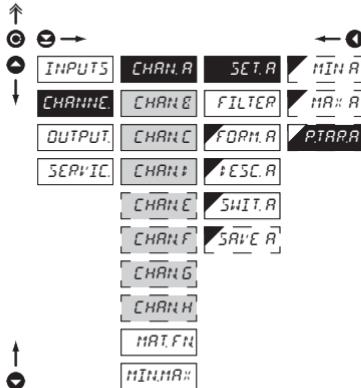 P.TARR.R


Setting "Fixed tare" value

- setting is designed for the event when it is necessary to firmly shift the beginning of the range by known size
- when setting [P. TAR. A > 0] display shows "T" symbol
- range of the setting is 0...9999
- **DEF** = 0

!

Setting is identical for input B, C, D, E, F, G, H

## 6.2.1c Digital filters

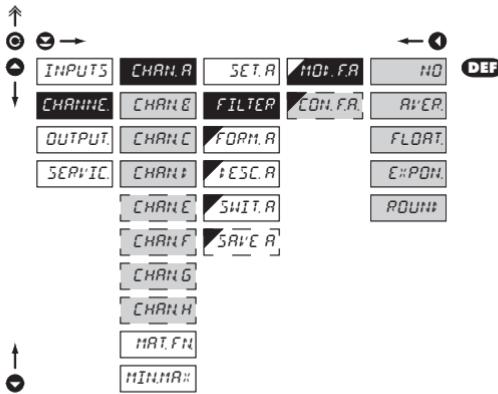

**MODE.F.R** Selection of digital filters

- at times it is useful for better user projection of data on display to modify it mathematically and properly, wherefore the following filters may be used:

**NO** Filters are off

**AVER.** Measured data average

- arithmetic average from given number („CON.F. A.“) of measured values
- range 2...100

**FLOAT.** Selection of floating filter

- floating arithmetic average from given number („CON.F. A.“) of measured data and updates with each measured value
- range 2...30

**EXPON.** Selection of exponential filter

- integration filter of first prvního grade with time constant („CON.F. A.“) measurement
- range 2...100

**ROUND** Measured value rounding

- is entered by any number, which determines the projection step (e.g.: "CON.F. A.=2,5 > display 0, 2,5, 5,...)


**CON.F.R.** Setting constants

- this menu item is always displayed after selection of particular type of filter
- **DEF** = 2

!

Setting is identical for input B, C, D, E, F, G, H

## 6.2.1d Projection format - positioning of decimal point

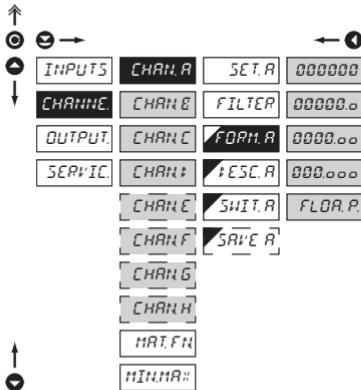

## FORM.R Selection of decimal point

- the instrument allows for classic projection of a number with positioning of the DP as well as projection with floating DP, allowing to display a number in its most exact form „FLOAT.P.“

**000000.** Setting DP - XXXX.

**00000.0** Setting DP - XXX.x

- **DEF**

**0000.00** Setting DP - XX.xx

**000.000** Setting DP - X.xxx


**FLOAT.P.**

Floating DP

!

Setting is identical for input B, C, D, E, F, G, H

## 6.2.1e Projection of description - the measuring units

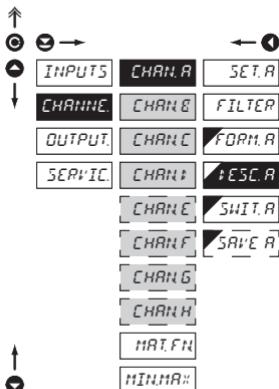


## #ESC.R Setting projection of descrip. for "Channel A"

- projection of measured data may be extended (at the expense of the number of displayed places) by two characters for description
- description is set by shifted ASCII code, where two first places show the set description and two last characters their code in period 0...95
- description is cancelled by code 00
- **RTD** **T/C** **DEF** = °C
- **DC** **PM** **DU** **OHM** **DEF** = none

!

Table of signs on page 89

## 6.2.1f Selection of channel projection upon switching

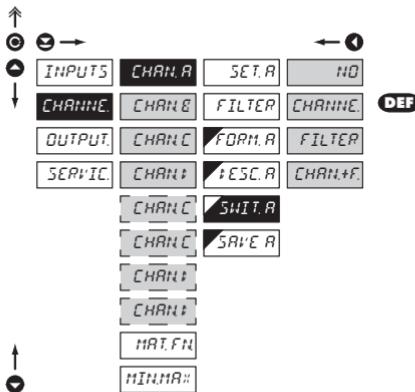

**SWITCH** Selection of channel projection upon switching

- setting in this item allows the user to choose individual measuring channels, which will be projected upon channel switching through function „SWITCH. A”

**NO** Projection prohibited

**CHANNEL A** "Channel A" will be projected


**FILTER** "Channel A" will be projected after digital filter modification

**CHAN.+F.** "Channel A" will be projected and subsequently also "Channel A" after digital filter modification

!

Setting is identical for input B, C, D, E, F, G, H

## 6.2.1g Selection of storing data into instrument memory

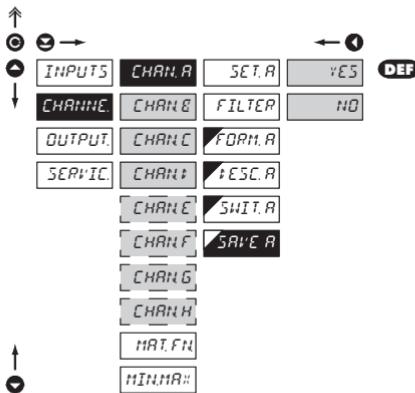

**SAVE** Selection of storing data into instrument memory

- by selection in this item you allow to register values into instrument memory  
- another setting in item "OUTPUT. > MEMORY" (not in standard experiment)


**YES** Measured data are stored in the memory

**NO** Measured data are not stored

!

Setting is identical for input B, C, D, E, F, G, H

## 6.2.2a Mathematic function - input selection

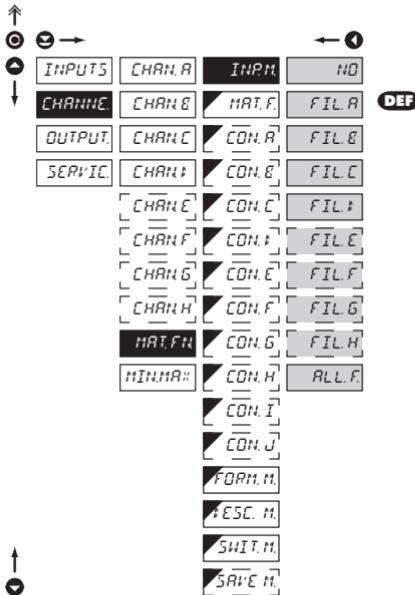
**INPM.** Selection of input for calculation of mat. function

- selection of value from which the mathematic function will be calculated

**NO** Mathematic functions are off

**FIL.R** From "input/channel A" after digital filter modification

**FIL.E** From "input/channel B" after digital filter modification

**FIL.C** From "input/channel C" after digital filter modification

**FIL.D** From "input/channel D" after digital filter modification

**FIL.E** From "input/channel E" after digital filter modification


**FIL.F** From "input/channel F" after digital filter modification

**FIL.G** From "input/channel G" after digital filter modification

**FIL.H** From "input/channel H" after digital filter modification

**ALL.F** From all inputs/channels after digital filter modification

## 6.2.2b Mathematic functions

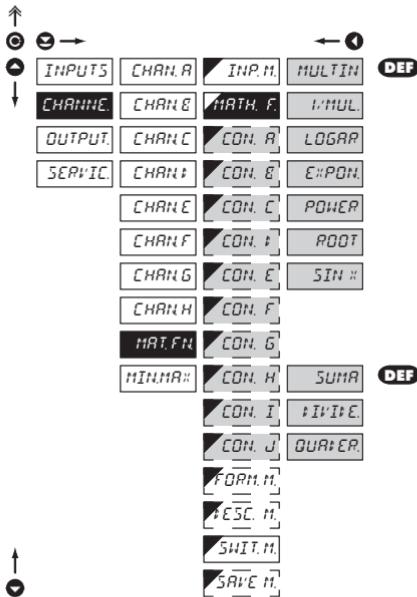

**MATH. F.** Selection of mathematic functions

In selecting „FIL.-“ in item „INP. M.“

**MULTIN** Polynome

$$Ax^5 + Bx^4 + Cx^3 + Dx^2 + Ex + F$$

**MMUL**  $1/x$

$$\frac{A}{x^3} + \frac{B}{x^4} + \frac{C}{x^3} + \frac{D}{x^2} + \frac{E}{x} + F$$

**LOGAR.** Logarithm

$$A \times \ln\left(\frac{Bx + C}{Dx + E}\right) + F$$

**EXPON.** Exponential

$$A \times e^{\left(\frac{Bx + C}{Dx + E}\right)} + F$$

**POWER** Power

$$A \times (Bx + C)^{(Dx+E)} + F$$

**ROOT** Root

$$A \times \sqrt{\frac{Bx + C}{Dx + E}} + F$$

**SIN X** Sin x

$$A \sin^5 x + B \sin^4 x + C \sin^3 x + D \sin^2 x + E \sin x + F$$

In selecting „ALL. F.“ in item „INP. M.“

**SUMMA** Total of values from channels (inputs)

$$(A \times KA + B \times KB + C \times KC + D \times KD + G \times KE + H \times KF + I \times KG + J \times KH) \times E + F$$

**DIVIDE** Channels (inputs) values division

$$(A \times KA + C \times KC + G \times KE + J \times KG) / (B \times KB + D \times KD + H \times KF + J \times KH) \times E + F$$

**QUATER.** Product of channels (inputs) values

$$(A \times KA^2 + B \times KB^2 + C \times KC^2 + D \times KD^2 + G \times KE^2 + H \times KF^2 + I \times KG^2 + J \times KH^2) \times E + F$$

**CON. -** Setting constants for calculation of mat. fce.

- this menu is displayed only after selection of given mathematic function

## 6.2.2c Mathematic functions - decimal point

INPUTS	CHAN A	INP.M.	000000
CHANNEL	CHAN B	MATH.F.	00000.0
OUTPUT	CHAN C	CON. A	0000.00
SERVICE	CHAN D	CON. B	000.000
	CHAN E	CON. C	FLOR.P.
	CHAN F	CON. D	
	CHAN G	CON. E	
	CHAN H	CON. F	
	MAT.FN	CON. G	
	MIN.MAX	CON. H	
		CON. I	
		CON. J	
		FORM.H	
		ESC. H.	
		SWIT.H.	
		SAVE H.	

**FORM.H.** Selection of decimal point

- the instrument allows for classic projection of a number with positioning of the DP as well as projection with floating DP, allowing to display a number in its most exact form „FLOR.P.”

000000 Setting DP - XXXX.

00000.0 Setting DP - XXX.x

0000.00 Setting DP - XX.xx

000.000 Setting DP - X.xxx

FLOR.P. Floating DP

- DEF

## 6.2.2d Mathematic functions - measuring units

INPUTS	CHAN A	MATH.F.	
CHANNEL	CHAN B	CON. A	
OUTPUT	CHAN C	CON. B	
SERVICE	CHAN D	CON. C	
	CHAN E	CON. D	
	CHAN F	CON. E	
	CHAN G	CON. F	
	CHAN H	FORM.H	
	MAT.FN	ESC. H.	
	MIN.MAX	SWIT.H.	
		SAVE H.	


**ESC.H.** Setting projection of description for "MAT.FN"

- projection of measured data may be extended (at the expense of the number of displayed places) by two characters for description
- description is set by shifted ASCII code, when two first places show the set description and two last characters their code in period 0...95
- description is cancelled by code 00
- DEF = no description

!

Table of signs on page 89

## 6.2.2e Mathematic functions - selection of channel projection upon switching

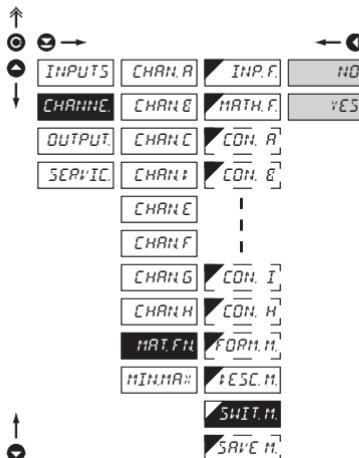


**SWIT.H.** Selection of channel projection upon switching

- setting in this item allows the user to chose individual measuring channels, which will get projected upon switching function channels „SWITCH. A“

YES Projection admitted

NO Projection denied

## 6.2.2f Mathematic functions - selection of storing data into instrument memory

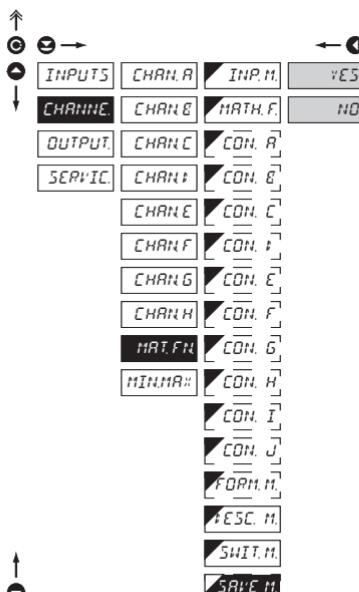


**SAVE.H.** Selection of storing data into instrument memory

- by selection in this item you allow to register values into instrument memory  
- another setting in item "OUTPUT. > MEMORY" (not in standard experiment)

YES Measured data are stored in the memory

NO Measured data are not stored

## 6.2.3 Selection of evaluation of min/max value

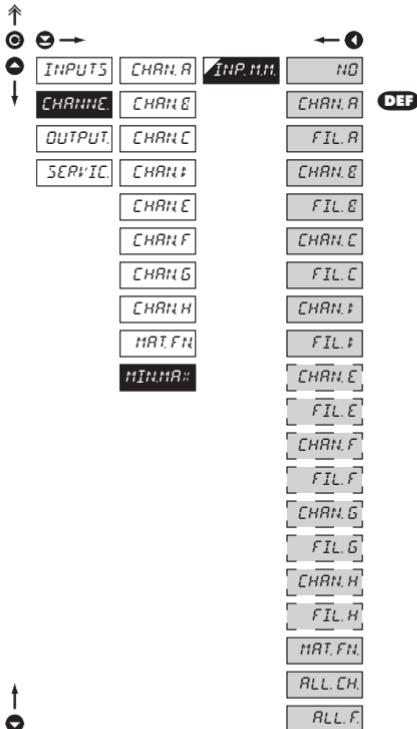 INP.MM. Selection of evaluation of min/max value

- selection of value from which the min/max value will be calculated

NO Evaluation of min/max value is off

CHAN.- From selected input

- selection from inputs 1, 2, 3, 4, 5, 6, 7, 8

FIL.- From selected input after digital filter modification


- selection from inputs 1, 2, 3, 4, 5, 6, 7, 8

MAT.FN. From "Mathematic functions"

ALL.CH. From all channels

ALL.F. From all inputs after digital filter modification

## 6.3 Setting „PROFI“ - OUTPUTS



In this menu it is possible to set parameters of the instrument output signals

**MEMORY** Setting data logging into memory


**LIMITS** Setting type and parameters of limits

**FTR** Setting type and parameters of data output

**AN. OUT** Setting type and parameters of analog output

**FISP.** Setting display projection and brightness

## 6.3.1a Selection of mode of data logging into instrument memory

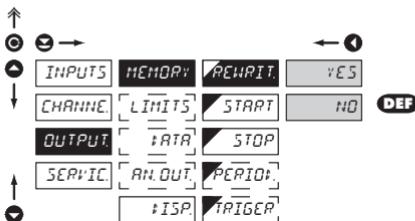


**REWRITE** Selection of the mode of data logging

- selection of the mode in the event of full instrument memory

**NO** Rewriting values prohibited

**YES** Rewriting values permitted, the oldest get rewritten by the latest

## 6.3.1b Setting data logging into instrument memory - RTC

**START**

Start of data logging into instrument memory

- time format HH.MM.SS

**STOP**

Stop data logging into instrument memory


- time format HH.MM.SS

**PERIOD**

Period of data logging into instrument memory

- determines the period in which values will be logged in an interval delimited by the time set under items START and STOP
- time format HH.MM.SS
- records are made on a daily basis in selected interval and period
- item not displayed if "STORE" is selected in menu (*Input > EXT. IN.*)

## 6.3.1c Setting data logging into instrument memory - FAST

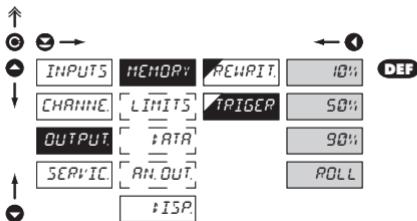**TRIGGER**

Setting logging data into inst. memory

- logging data into inst. memory is governed by the following selection, which determines how many percent of the memory is reserved for data logging prior to initiation of trigger impulse
- initiation is on ext. input or control key

10%

Reser. of 10 % memory  
prior init. of data logging

50%

Reser. of 50 % memory  
prior init. of data logging

90%

Reser. of 90 % memory  
prior init. of data logging

ROLL

After initiation of data  
logging the memory is  
cyclically transcribed


## 6.3.2a Selection of input for limits evaluation

Inputs for limit evaluation:

INPUTS	MEMORY	LIM 1	INP.LI	NO
CHANNEL	LIMITS	LIM 2	HOF.LI	CHAN.R
OUTPUT	FTR	LIM 3	TYP.LI	FIL.R
SERVICE	RN.OUT	LIM 4	LIM.LI	CHAN.E
	#ISP	LIM 5	HYS.LI	FIL.E
		LIM 6	ON.LI	CHAN.E
		LIM 7	OFF.LI	FILE
		LIM 8	PER.LI	CHAN.I
			THL.LI	FIL.I
			CHAN.E	
			FIL.E	
			CHAN.F	
			FIL.F	
			CHAN.G	
			FIL.G	
			CHAN.H	
			FIL.H	
			MAT.FN	
			MIN	
			MAX	
			ALL.CH.	
			ALL.F.	

<input checked="" type="checkbox"/> INP.LI Selection evaluation of limits	
- selection of value from which the limit will be evaluated	
<input type="checkbox"/> NO	Limit evaluation is off
<input type="checkbox"/> CHAN.-	From selected input
-	selection from inputs 1, 2, 3, 4, 5, 6, 7, 8
<input type="checkbox"/> FIL.-	From selected input after digital filter modification
-	selection from inputs 1, 2, 3, 4, 5, 6, 7, 8
<input type="checkbox"/> MAT.FN	Limit evaluation from "Mathematic functions"
<input type="checkbox"/> MIN	Limit evaluation from "Min.value"
<input type="checkbox"/> MAX	Limit evaluation from "Max.value"
<input type="checkbox"/> ALL.CH.	From all inputs
<input type="checkbox"/> ALL.F.	From all inputs after digital filter modification
<b>!</b>	
Setting is identical for UM 2 ... UM 8	

## 6.3.2b Selection of type of limit

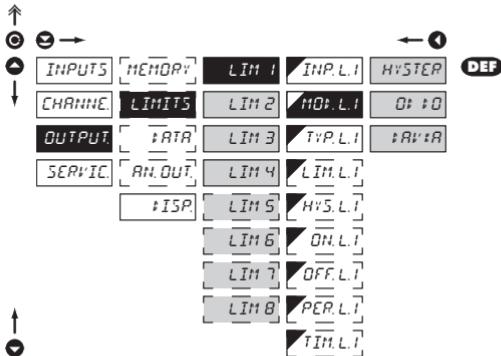 **MFL.I** Selection the type of limit

**HYS.L.I** Limit is in mode "Limit, hysteresis, delay"

- for this mode the parameters of "LIM. L." are set, at which the limit will shall react, "HYS. L." the hysteresis range around the limit ( $LIM \pm 1/2 HYS$ ) and time "TIM. L." determining the delay of relay switch-on

**FROM.** Frame limit

- for this mode the parameters are set for interval "ON. L." the relay switch-on and "OFF. L." the relay switch-off


**FOSING** Dose limit  
(periodic)

- for this mode the parameters are set for "PER. L." determining the limit value as well as its multiples at which the output is active and "TIM. L." indicating the time during which is the output active



Setting is identical for LIM 2 ... LIM 8

## 6.3.2c Selection of type of output

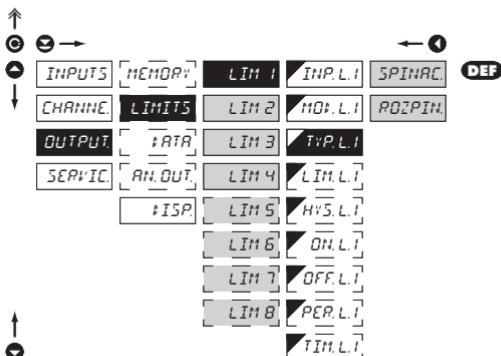 **TVPL.I** Selection of type of output

**CLOSE.**

Output switches on when condition is met


**OPEN**

Output switches off when condition is met



Setting is identical for LIM 2 ... LIM 8

## 6.3.2d Setting values for limits evaluation

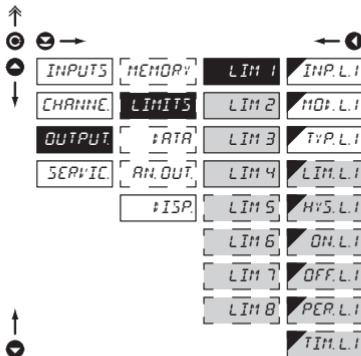

**LIM.L.I** Setting limit for switch-on

- for type "HYSTER"

**HYS.L.I** Setting hysteresis

- for type "HYSTER"

- indicates the range around the limit (in both directions, LIM.  $\pm 1/2$  HYS.)

**ON.L.I** Setting the outset of the interval of limit switch-on

- for type "FROM"

**OFF.L.I** Setting the end of the interval of limit switch-on

- for type "FROM"

**PER.L.I** Setting the period of limit switch-on

- for type "DOSE"


**TIM.L.I** Setting the time switch-on of the limit

- for type "HYSTER" and "DOSE"

!


Setting is identical for LIM 2 ... LIM 8

## 6.3.3a Selection of data output baud rate

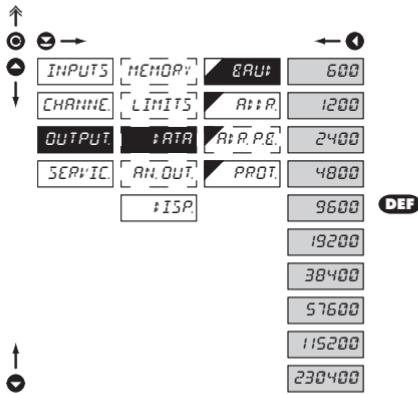

Selection of data output baud rate	
600	Rate - 600 Baud
1200	Rate - 1 200 Baud
2400	Rate - 2 400 Baud
4800	Rate - 4 800 Baud
9600	Rate - 9 600 Baud
19200	Rate - 19 200 Baud
38400	Rate - 38 400 Baud
57600	Rate - 57 600 Baud
115200	Rate - 115 200 Baud
230400	Rate - 230 400 Baud

## 6.3.3b Setting instrument address



Setting instrument address	
- setting in range 0...31	
- DEF = 00	

Setting instrument address - MODBUS	
- setting in range 1...247	
- DEF = 1	

## 6.3.3c Selection of data output protocol

**INPUTS** [MEMORY] **BAUD** **RSCII** **DEF**  
**CHANNEL** [LIMITS] **RTT.R.** **MESUS**  
**OUTPUT** **#RTA** **RTT.PE** **MOBUS**  
**SERVICE** **RN OUT** **PROT.**  
**#ISP.**

 **PROT.** Selection of the type of analog output

**RSCII** Data protocol ASCII

**MESUS** Data protocol DIN MessBus

**MOBUS** Data protocol MODBUS-RTU

- option is available only for RS 485

## 6.3.4a Selection of input for analog output

**INPUTS** [MEMORY] **INP.RD** **NO** **DEF**  
**CHANNEL** [LIMITS] **TYP.RD** **CHAN.R**  
**OUTPUT** **#RTA** **MIN.RD** **FIL.R**  
**SERVICE** **RN OUT** **MAX.RV** **CHAN.E**  
**#ISP.** **FIL.E**  
**CHAN.E**  
**FIL.E**  
**CHAN.F**  
**FIL.F**  
**CHAN.G**  
**FIL.G**  
**CHAN.H**  
**FIL.H**  
**MAT.FN**  
**MIN**  
**MAX**  
**#ISPL.**

 **INP.RD** Selection evaluation analog output

- selection of value from which the analog output will be evaluated

**NO** AO evaluation is off

**CHAN.-** From selected input

- selection from inputs 1, 2, 3, 4, 5, 6, 7, 8

**FIL.-** From selected input after digital filter modification

- selection from inputs 1, 2, 3, 4, 5, 6, 7, 8


**MAT.FN** AO evaluation from "Math.functions"

**MIN** AO evaluation from "Min.value"

**MAX** AO evaluation from "Max.value"

**#ISPL.** From currently displayed value

## 6.3.4b Selection of the type of analog output

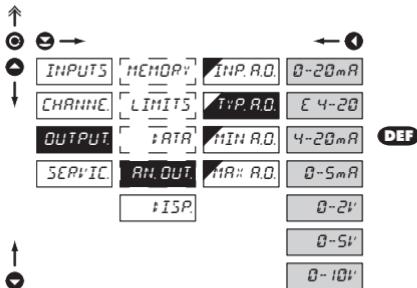

## TYP. R.O. Selection of the type of analog output

0-20mA Type - 0...20 mA

E 4-20 Type - 4...20 mA

- with indication of error statement (&lt; 3,0 mA)

4-20mA Type - 4...20 mA


0-5mA Type - 0...5 mA

0-2V Type - 0...2 V

0-5V Type - 0...5 V

0-10V Type - 0...10 V

## 6.3.4c Setting the analog output range



## AN. OUT. Setting the analog output range

- analog output is isolated and its value corresponds with displayed data. It is fully programmable, i.e. it allows to assign the AO limit points to two arbitrary points of the entire measuring range

**MIN R.O.** Assigning the display value to the beginning of the AO range

- range of the setting is -999...9999


- **DEF** = 0

**MR:: R.O.** Assigning the display value to the end of the AO range

- range of the setting is -999...9999


- **DEF** = 100

## 6.3.5a Selection of input for display projection

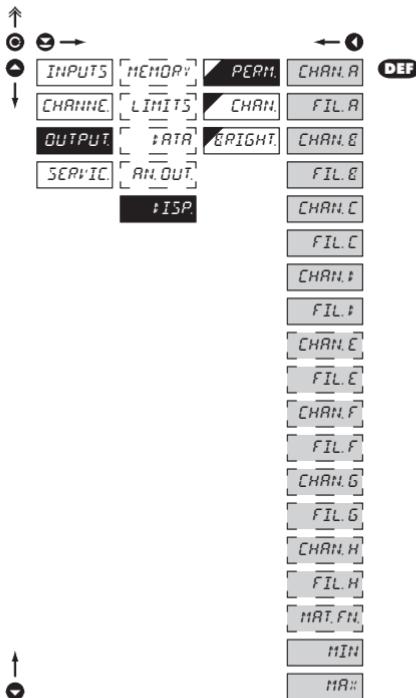

PERM. Selection display projection	
-	selection of value which will be shown on the instrument display
<input type="checkbox"/> <b>CHAN.R</b>	Projection of values from "Channel A"
<input type="checkbox"/> <b>FIL.R</b>	From "Channel A" after digital filters processing
<input type="checkbox"/> <b>CHAN.E</b>	Projection of values from "Channel B"
<input type="checkbox"/> <b>FIL.E</b>	From "Channel B" after digital filters processing
<input type="checkbox"/> <b>CHAN.C</b>	Projection of values from "Channel C"
<input type="checkbox"/> <b>FIL.C</b>	From "Channel C" after digital filters processing
<input type="checkbox"/> <b>CHAN.D</b>	Projection of values from "Channel D"
<input type="checkbox"/> <b>FIL.D</b>	From "Channel D" after digital filters processing
<input type="checkbox"/> <b>CHAN.E</b>	Projection of values from "Channel E"
<input type="checkbox"/> <b>FIL.E</b>	From "Channel E" after digital filters processing
<input type="checkbox"/> <b>CHAN.F</b>	Projection of values from "Channel F"
<input type="checkbox"/> <b>FIL.F</b>	From "Channel F" after digital filters processing
<input type="checkbox"/> <b>CHAN.G</b>	Projection of values from "Channel G"
<input type="checkbox"/> <b>FIL.G</b>	From "Channel G" after digital filters processing
<input type="checkbox"/> <b>CHAN.H</b>	Projection of values from "Channel H"
<input type="checkbox"/> <b>FIL.H</b>	From "Channel H" after digital filters processing
<input type="checkbox"/> <b>MAT.FN.</b>	Projection of values from "Math.functions"
<input type="checkbox"/> <b>MIN</b>	Projection of values from "Min.value"
<input type="checkbox"/> <b>MAX</b>	Projection of values from "Max.value"

## 6.3.5b Selection of signalization of measuring inputs on display

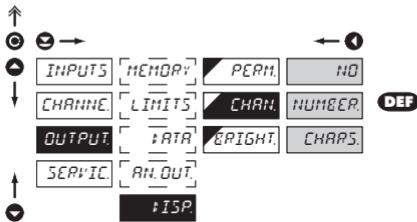 **CHAN.** Selection of inputs signalization

**NO** Display is off


**NUMBER** Numeric description of inputs

- inputs are marked 1, 2, 3, 4, 5, 6, 7, 8

**CHARS** Alphabetical description of inputs

- inputs are marked A, B, C, D, E, F, G, H

## 6.3.5c Selection of display brightness

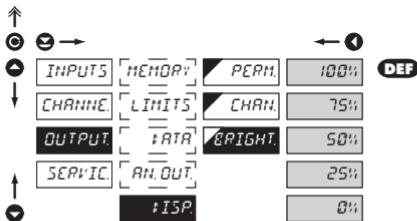 **ERIGHT** Selection of display brightness

- by selecting display brightness we may appropriately react to light conditions in place of instrument location

**0%** Display is off

- after keystroke display turns on for 10 s


**25%** Display brightness - 25 %

**50%** Display brightness - 50 %

**75%** Display brightness - 75 %

**100%** Display brightness - 100 %


## 6.4 Setting "PROFI" - SERVICE



The instrument service functions are set in this menu

<b>MENU</b>	Selection of menu type LIGHT/PROFI
<b>RESTOR.</b>	Restore instrument manufacture setting and calibration
<b>CALIB.</b>	Input range calibration for „DU“ version
<b>LANG.</b>	Language version of instrument menu
<b>N.PASS.</b>	Setting new access password
<b>IDENT.</b>	Instrument identification

## 6.4.1 Selection of type of programming menu

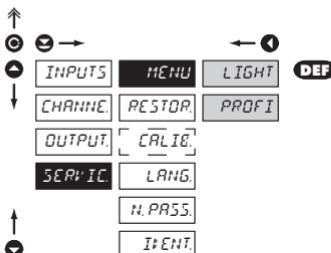**MENU** Selection of menu type - LIGHT/PROFI

- enables setting the menu complexity according to user needs and skills

**LIGHT** Active LIGHT menu

- simple programming menu, contains only items necessary for configuration and instrument setting
- linear menu > items one after another



**PROFI** Active PROFI menu

- complete programming menu for expert users
- tree menu



Change of setting is valid upon next access into menu

## 6.4.2 Restoration of manufacture setting

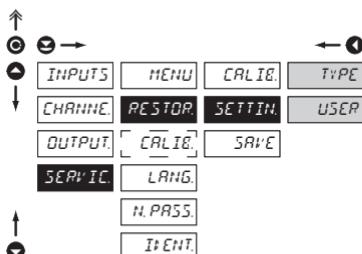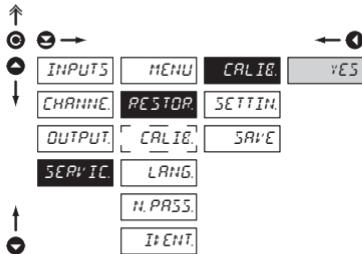**RESTOR.** Restoration of manufacture setting

- in the event of error setting or calibration, manufacture setting may be restored.

**CALIB.** Restoration of manufacture calibration of the instrument

- prior executing the changes you will be asked to confirm your selection „YES”

**SETTIN.** Restoration of instrument manufacture setting

**TYPE** Restoration of instrument manufacture setting

- generating the manufacture setting for currently selected type of instrument (items marked DEF)

**USER** Restoration of instrument user setting

- generating the instrument user setting, i.e. setting stored under SERVICE./RESTOR./SAVE

**SAVE** Save instrument user setting

- storing the user setting allows the operator to restore it in future if needed


Jobs performed	Restore	
	Calibration	Setting
cancels USER menu rights	✓	✓
deletes table of items order in USER - LIGHT menu	✓	✓
adds items from manufacture to LIGHT menu	✓	✓
deletes data stored in FLASH	✓	✓
cancels or linearization tables	✓	✓
clears tare	✓	✓
clears conduct resistances	✓	✓
restore manufacture calibration	✓	✗
restore manufacture setting	✗	✓



After restoration the instrument switches off for couple seconds

## 6.4.3

## Calibration - Input range

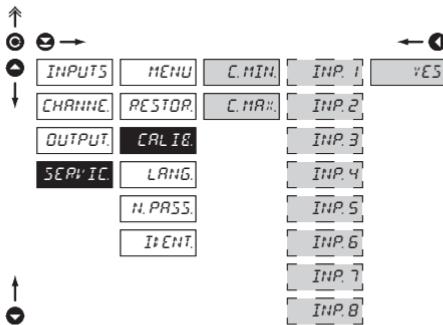


## CALIB. Input range calibration

- the inputs for calibration always include only active inputs, i.e. those that are set for "MOD > DU".
- after projection of "C. MIN." and selection of relevant input move the potentiometer runner into required minimum position and confirm by „Enter”, calibration is confirmed by „YES” notice
- after projection of "C. MAX." and selection of given input move the potentiometer into required maximum position and confirm by „Enter”, calibration is confirmed by „YES”

## 6.4.4


## Selection of instrument menu language version

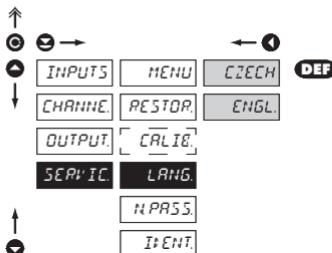

## LANG. Selection of instrument menu language version

- |       |                               |
|-------|-------------------------------|
| CZECH | Instrument menu is in Czech   |
| ENGL. | Instrument menu is in English |


## 6.4.5 Setting new access password



**N.PASS.** Setting new password  
for access to LIGHT  
and PROFI menu

- this selection enables changing number code that blocks the access into LIGHT and PROFI Menu.
- range of the number code is 0...9999
- universal password in the event of loss is „8177”

## 6.4.6 Instrument identification




**IDENT.** Projection of instrument  
SW version

- display shows type identification of the instrument, SW number, SW version and current input setting (Mode)
- if the SW version reads a letter on first position, it is a customer SW

## 7.0 Setting items into "USER" menu

- **USER** menu is designed for users who need to change only several items of the setting without the option to change the primary instrument setting (e.g. repeated change of limit setting)
- there are no items from manufacture permitted in **USER** menu
- on items indicated by inverse triangle  *L*
- setting may be performed in **LIGHT** or **PROFI** menu, with the **USER** menu then overtaking the given menu structure

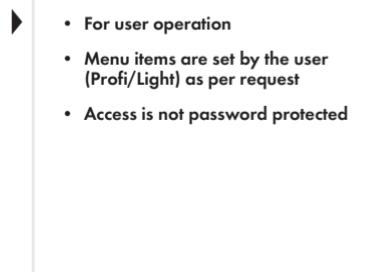

## Setting

**NO**

item will not be displayed in USER menu

**YES**

item will be displayed in USER menu with editing option

**SHOW**

item will be solely displayed in USER menu

**Setting sequence of items in "USER" menu**

In compiling USER menu from active LIGHT menu the items (max. 10) may be assigned a sequence, in which they will be projected in the menu

**Example:**

Into USER menu were selected these items


(keys + > CL. TAR., LIM 1, LIM 2, LIM 3, for which we have preset this sequence (keys + ):

CL. TAR.	5
LIM 1	0 (sequence not determined)
LIM 2	2
LIM 3	1

Upon entering USER menu

(key items will be projected in the following sequence: LIM 3 > LIM 2 > CL.TAR. > LIM 1

Instrument with input for temperature measurement with thermocouple allows to set two types of measurement of cold junction.

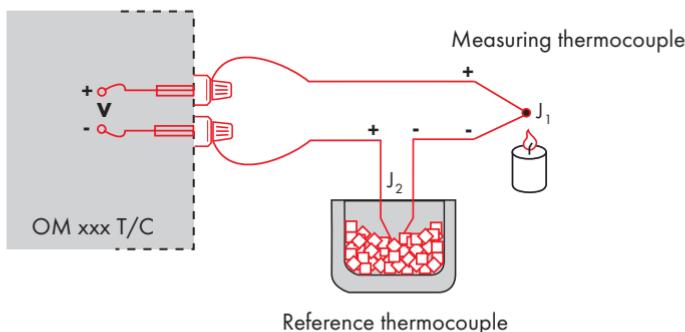

#### WITH REFERENCE THERMOCOUPLE

- a reference thermocouple may be located in the same place as the measuring instrument or in place with stable temperature/compensation box
- when measuring with reference thermocouple set *CONECT* in the instrument menu to *INT2TC* or *E<sub>2</sub>T2TC*
- when using a thermostat (a compensation box or environment with constant temperature) set in the instrument menu *CJC,TET*, its temperature (applies for setting *CONECT* to *E<sub>2</sub>T2TC*)
- if the reference thermocouple is located in the same environment as the measuring instrument then set in the instrument menu *CONECT* to *INT2TC*. Based on this selection the measurement of the ambient temperature is performed by a sensor located in the instrument terminal board.

#### WITHOUT REFERENCE THERMOCOUPLE

- inaccuracy originating from the creation of dissimilar thermocouples on the transition point terminal/conductor of the thermocouple is not compensated for in the instrument
- when measuring without reference thermocouple set *CONECT* in the instrument menu to *INT,ITE* or *E<sub>2</sub>T,ITE*
- when measuring temperature without reference thermocouple the error in measured data may be as much as 10°C (applies for setting *CONECT* to *E<sub>2</sub>T,ITE*)



The instruments communicate via serial line RS232 or RS485. For communication they use the ASCII protocol. Communication runs in the following format:

ASCII: 8 bit, no parity, one stop bit  
 DIN MessBus: 7 bit, even parity, one stop bit

The transfer rate is adjustable in the instrument menu. The instrument address is set in the instrument menu in the range of 0 ÷ 31. The manufacture setting always presets the ASCII protocol, rate of 9600 Baud, address 00. The type of line used - RS232 / RS485 - is determined by an output board automatically identified by the instrument.

The commands are described in specifications you can find at [www.orbit.merret.cz/rs](http://www.orbit.merret.cz/rs) or in the OM Link program.

#### DETAILED DESCRIPTION OF COMMUNICATION VIA SERIAL LINE

Event	Type	Protocol	Transmitted data											
Data solicitation (PC)	232	ASCII	#	A	A	<CR>								
		MessBus	No - data is transmitted permanently											
	485	ASCII	#	A	A	<CR>								
		MessBus	<SADR>	<ENQ>										
Data transmission (instrument)	232	ASCII	>	D	(D)	(D)	(D)	(D)	(D)	(D)	(D)	(D)	<CR>	
		MessBus	<SADR>	D	(D)	(D)	(D)	(D)	(D)	(D)	(D)	(D)	<ETX>	<BCC>
	485	ASCII	>	D	(D)	(D)	(D)	(D)	(D)	(D)	(D)	(D)	<CR>	
		MessBus	<SADR>	D	(D)	(D)	(D)	(D)	(D)	(D)	(D)	(D)	<ETX>	<BCC>
Confirmation of data acceptance (PC) - OK	485	MessBus	<DLE>	1										
Confirmation of data acceptance (PC) - Bad			<NAK>											
Sending address (PC) prior command			<EADR>	<ENQ>										
Confirmation of address (instrument)			<SADR>	<ENQ>										
Command transmission (PC)	232	ASCII	#	A	A	N	P	(D)	(D)	(D)	(D)	(D)	(D)	<CR>
		MessBus	<STX>	\$	N	P	(D)	(D)	(D)	(D)	<ETX>	<BCC>		
	485	ASCII	#	A	A	N	P	(D)	(D)	(D)	(D)	(D)	(D)	<CR>
		MessBus	<SADR>	\$	N	P	(D)	(D)	(D)	(D)	<ETX>	<BCC>		
Command confirmation (instrument)	232	ASCII	OK	!	A	A	<CR>							
		Bad	?	A	A	<CR>								
	485	MessBus	No - data is transmitted permanently											
			OK	I	A	A	<CR>							
			Bad	?	A	A	<CR>							
			OK	<DLE>	1									
			Bad	<NAK>										
Command confirmation (inst.) - OK	485	MessBus	!	A	A	<CR>								
Command confirmation (instrument) - Bad			?	A	A	<CR>								
Instrument identification			#	A	A	1Y	<CR>							
HW identification			#	A	A	1Z	<CR>							
One-time transmission			#	A	A	7X	<CR>							
Repeated transmission			#	A	A	8X	<CR>							

**LEGEND**

	#	35	23 <sub>H</sub>	Command beginning
A	A	0...31	0D <sub>H</sub>	Two characters of instrument address (sent in ASCII - tens and units, e.g. "01", "99" universal)
<CR>	13	0D <sub>H</sub>		Carriage return
<SP>	32	20 <sub>H</sub>		Space
N, P				Number and command - command code
D				Data - usually characters "0"..."9", ".", "; (D) - dp. and (;) may prolong data
R	30 <sub>H</sub> ...3F <sub>H</sub>			Relay and tare status
!	33	21 <sub>H</sub>		Positive confirmation of command (ok)
?	63	3F <sub>H</sub>		Negative confirmation of command (point)
>	62	3E <sub>H</sub>		Beginning of transmitted data
<STX>	2	02 <sub>H</sub>		Beginning of text
<ETX>	3	03 <sub>H</sub>		End of text
<SADR>	addressa	+60 <sub>H</sub>		Prompt to send from address
<EADR>	addressa	+40 <sub>H</sub>		Prompt to accept command at address
<ENQ>	5	05 <sub>H</sub>		Terminate address
<DLE>1	16	10 <sub>H</sub>		Confirm correct statement
	49	31 <sub>H</sub>		
<NAK>	21	15 <sub>H</sub>		Confirm error statement
<BCC>				Check sum -XOR

**RELAY, TARE**

Sign	Relay 1	Relay 2	Tare	Change relay 3/4
P	0	0	0	0
Q	1	0	0	0
R	0	1	0	0
S	1	1	0	0
T	0	0	1	0
U	1	0	1	0
V	0	1	1	0
W	1	1	1	0
p	0	0	0	1
q	1	0	0	1
r	0	1	0	1
s	1	1	0	1
t	0	0	1	1
u	1	0	1	1
v	0	1	1	1
w	1	1	1	1

Relay status is generated by command #AA6X <CR>.

The instrument immediately returns the value in the format >HH <CR>, where HH is value in HEX format and range 00<sub>H</sub>...FF<sub>H</sub>. The lowest bit stands for „Relay 1”, the highest for „Relay 8”

ERROR	CAUSE	ELIMINATION
<i>E.I.U.</i>	Number is too small (large negative) to be displayed	change DP setting, channel constant setting
<i>E.I.O.</i>	Number is too large to be displayed	change DP setting, channel constant setting
<i>E.T.U</i>	Number is outside the table range	increase table values, change input setting (channel constant setting)
<i>E.T.O.</i>	Number is outside the table range	increase table values, change input setting (channel constant setting)
<i>E.I.U.</i>	Input quantity is smaller than permitted input quantity range	change input signal value or input (range) setting
<i>E.I.O.</i>	Input quantity is larger than permitted input quantity range	change input signal value or input (range) setting
<i>E.HW</i>	A part of the instrument does not work properly	send the instrument for repair
<i>E.EE</i>	Data in EEPROM corrupted	perform restoration of manufacture setting, upon repeated error statement send instrument for repair
<i>E.FATA</i>	Data in EEPROM outside the range	perform restoration of manufacture setting, upon repeated error statement send instrument for repair
<i>E.CLR</i>	Memory was empty (presetting carried out)	upon repeated error statement send instrument for repair, possible failure in calibration

The instrument allows to add two descriptive characters to the classic numeric formats (at the expense of the number of displayed places). The setting is performed by means of a shifted ASCII code. Upon modification the first two places display the entered characters and the last two places the code of the relevant symbol from 0 to 95. Numeric value of given character equals the sum of the numbers on both axes of the table.

Description is cancelled by entering characters with code 00

	0	1	2	3	4	5	6	7	0	1	2	3	4	5	6	7	
0	!	"	#	\$	%	&	'		!	"	#	\$	%	&	'		
8	:	,	*	+	,	-	,	8	(	)	*	+	,	-	.	/	
16	0	1	2	3	4	5	6	7	16	0	1	2	3	4	5	6	7
24	8	9	"	"	(	)	-	7	24	8	9	:	;	<	=	>	?
32	P	R	E	C	A	E	F	G	32	@	A	B	C	D	E	F	G
40	H	I	J	K	L	M	N	O	40	H	I	J	K	L	M	N	O
48	P	Q	R	S	T	U	V	W	48	P	Q	R	S	T	U	V	W
56	X	Y	Z	C	\	]	^	-	56	X	Y	Z	[	\	^	-	
64	'	a	b	c	d	e	F	G	64	'	a	b	c	d	e	f	g
72	h	i	j	k	l	m	n	o	72	h	i	j	k	l	m	n	o
80	P	Q	r	s	t	u	v	w	80	p	q	r	s	t	u	v	w
88	X	Y	Z	\	/	~	o		88	x	y	z	{		}	~	



**DATA OUTPUTS**

Protocols:	ASCII, DIN MessBus, MODBUS, PROBUS
Data format:	8 bit + no parity + 1 stop bit (ASCII) 7 bit + even parity + 1 stop bit (MessBus)
Rate:	600...230 400 Baud
RS 232:	isolated, two-way communication
RS 485:	isolated, two-way communication, addressing (max. 31 instruments)
PROFIBUS	Data protocol SIEMENS

**ANALOGO OUTPUTS**

Type:	isolated, programmable with resolution of max.10 000 points, analog output corresponds with displayed data, type and range are adjustable
Non-linearity:	0.2 % of range
TC:	100 ppm/°C
Rate:	response to change of value < 150 ms
Voltage:	0...2 V/5 V/10 V
Current:	0...5/20 mA/4...20 mA - compensation of conduct to 500 Ohm/12 V or 1 000 Ohm/24 V

**MEASURED DATA RECORD**

Type RTC:	time-controlled logging of measured data into instrument memory, allows to log up to 250 000 values
Type FAST:	fast data logging into instrument memory, allows to log up to 8 000 values at a rate of 40 records/s
Transmission:	via data output RS 232/485 or via OM Link

**POWER SUPPLY**

Options:	10...30 V AC/DC, 10 VA, isolated, - fuse inside (T 4000 mA) 80...250 V AC/DC, 10 VA, isolated - fuse inside (T 630 mA)
----------	---

**MECHANIC PROPERTIES**

Material:	Noryl GFN2 SE1, incombustible UL 94 V-I
Dimensions:	96 x 48 x 120 mm
Panel cut-out:	90,5 x 45 mm

**OPERATING CONDITIONS**

Connection:	connector terminal board, conductor cross-section <1,5 mm <sup>2</sup> />2,5 mm <sup>2</sup>
Stabilisation period:	within 15 minutes after switch-on
Working temp.:	0°...60°C
Storage temp.:	-10°...+85°C
Cover:	IP65 (front panel only)
Construction:	safety class I
Overvoltage category:	EN 61010-1, A2
Insulation resistance:	for pollution degree II, measurement category III instrum.power supply > 670 V (PI), 300 V (DI) Input/output > 300 V (PI), 150 (DI)
EMC:	EN 61000-3-2+A12; EN 61000-4-2, 3, 4, 5, 8, 11; EN 550222, A1, A2

*\*\*Table of measuring rate on one channel, according to setting of input mode and type of measurement*

<b>Channels/Rate</b>	<b>40</b>	<b>20</b>	<b>10</b>	<b>5</b>	<b>2</b>	<b>1</b>	<b>0,5</b>	<b>0,2</b>	<b>0,1</b>
<i>Input mode &gt; SWITCH - single channel measurement</i>	40,00	20,00	10,00	5,00	2,00	1,00	0,50	0,20	0,10
<i>Input mode &gt; SWITCH - dual channel measurement</i>	6,667	3,333	1,667	1,25	0,714	0,417	0,227	0,096	0,049
<i>Input mode &gt; CYCLE - 2x single channel meas.</i>	6,667	3,333	1,667	1,25	0,714	0,417	0,227	0,096	0,049
<i>Input mode &gt; CYCLE - 1x single + 1x dual channel measurement</i>	4,444	2,222	1,111	0,833	0,476	0,278	0,152	0,064	0,033
<i>Input mode &gt; CYCLE - 2x dual channel measurement</i>	3,333	1,667	0,833	0,625	0,357	0,208	0,114	0,048	0,025



*Measuring rate in the menu is indicated for mode SWITCH and single channel measurement.*

*Single channel measurement > DC, PM, DU, OHM - 2/4 wire, Pt - 2/4 wire, Ni - 2/4 wire, Cu - 2/4 wire, TC on 1st input with external compensation, TC on other inputs*

*Dual channel measurement > OHM - 3 wire, Pt - 3 wire, Ni - 3 wire, Cu - 3 wire, TC on 1st input with internal compensation*

*If at least one TC measurement with internal compensation is to be used, IT HAS TO BE connected on 1st input. Cold junction value is measured here!*



*The instrument contains up to 4 A/D converters that always control one pair of inputs 1.+2., 3.+4., 5.+6., 7.+8. Converters measure almost simultaneously.*

**Front view****Panel cut****Side view**

Panel thickness: 0,5...20 mm

#### **Instrument installation**

1. insert the instrument into the panel cut-out
2. fit both travellers on the box
3. press the travellers close to the panel

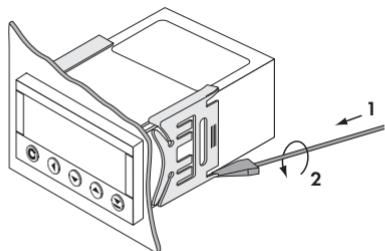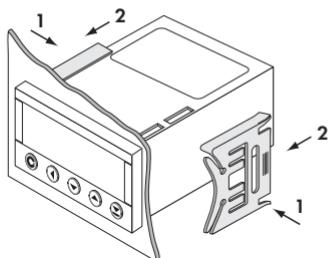

#### **Instrument disassembly**

1. slide a screw driver under the traveller wing
2. turn the screw driver and remove the traveller
3. take the instrument out of the panel

Product                   **OMU 408**

Type .....

Manufacturing No. .....

Date of sale .....

# GUARANTEE

A guarantee period of 60 months from the date of sale to the user applies to this instrument.

Defects occurring during this period due to manufacture error or due to material faults shall be eliminated free of charge.

For quality, function and construction of the instrument the guarantee shall apply provided that the instrument was connected and used in compliance with the instructions for use.

The guarantee shall not apply to defects caused by:

- mechanic damage
- transportation
- intervention of unqualified person incl. the user
- unavoidable event
- other unprofessional interventions

The manufacturer performs guarantee and post-guarantee repairs unless provided for otherwise.

Y E A R S

Stamp, signature

## NOTE



# DECLARATION OF CONFORMITY

**Company:****ORBIT MERRET, spol. s r.o.**

Klánová 81/141, 142 00 Prague 4, Czech Republic, IDNo: 00551309

**Manufactured:****ORBIT MERRET, spol. s r.o.**

Vodňanská 675/30, 198 00 Prague 9, Czech Republic

declares at its full responsibility that the product presented hereunder meets all technical requirements, is safe for use when utilised under the terms and conditions determined by ORBIT MERRET, spol.s.r.o. and that our company has taken all measures to ensure conformity of all products of the type listed hereunder, which are being brought out to the market, with technical documentation and requirements of the appurtenant statutory orders.

**Product:**

4-digit programmable panel instrument

**Type:****OMU 408**Conformity is assessed pursuant to the following standards:

El. safety:	EN 61010-1
EMC:	EN 50131-1, chapter 14 and chapter 15
	EN 50130-4, chapter 7 EN 61000-4-11
	EN 50130-4, chapter 8 EN 61000-4-11
	EN 50130-4, chapter 9 EN 61000-4-2
	EN 50130-4, chapter 10 EN 61000-4-3
	EN 50130-4, chapter 11 EN 61000-4-6
	EN 50130-4, chapter 12 EN 61000-4-4
	EN 50130-4, chapter 13 EN 61000-4-5
	EN 50130-5, chapter 20
	prEN 50131-2-1, par. 9.3.1
	EN 61000-4-8
	EN 61000-4-9
	EN 61000-3-2 ed. 2:2001
	EN 61000-3-3: 1997, Cor. 1:1998, Z1:2002
	EN 55022, chapter 5 and chapter 6

and Ordinance on:

El. safety:	No. 168/1997 Coll.
EMC:	No. 169/1997 Coll.

The evidence are the protocols of authorized and accredited organizations:

VTÚE Praha, experimental laboratory No. 1158, accredited by ČIA

VTÚPV Vyškov, experimental laboratory No. 1103, accredited by ČIA

Place and date of issue:

Prague, 18. March 2006

Miroslav Hackl v.r.

Company representative

Mode of asses. of conformity §12, par. 4 b, d Act No. 22/1997 Coll.

TECHDOK - OMU 408 - 2007 - 1v1 - en - V