



OMX 103UNI




- 2x multifunction input (DC, PM, RTD, T/C, DU)
- LCD display, Digit. filters, Tare, Linearization
- 3x Card slots
- Galvanic separation 2.5 kVAC
- Power supply 10...30 V AC/DC; 80...250 V AC/DC

Option

Comparators ● Data output ● Data record

PROGRAMMABLE ISOLATED TRANSMITTER

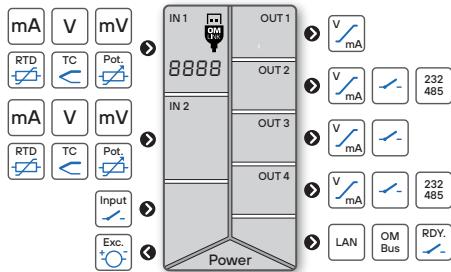

OPERATION

The instrument is set and controlled by two buttons located on the front panel. All programmable settings of the instrument may be performed in three adjusting modes:

LIGHT MENU is protected by an optional number code and contains solely items necessary for instrument setting.

PROFI MENU is protected by an optional number code and contains complete instrument setting.

USER MENU may contain arbitrary items from the programming menu (LIGHT/PROFI), which determine the access rights (see, change). Access w/o password.

Standard equipment is the OM Link and USB interfaces, which together with operation program enables modification and filing of all instrument settings as well as performing firmware updates. The program is also designed for visualization and filing of measured values from more instruments.

The measured units can be projected on the display.

OPTIONS

COMPARATORS are assigned to monitor six limit values with relay output. The limits have adjustable hysteresis within the full range of the display as well as selectable delay of the switch-on in the range of 0...99.9 s. Reaching the preset limits is signalled by LED and simultaneously by the switch-on of the relevant relay.

ANALOG OUTPUTS will find their place in applications where further evaluating or processing of measured data is required in external devices. We offer universal analog output with the option of selection of the type of output - voltage/current. The value of analog output corresponds with the displayed data. Its type and range are selectable in menu.

DATA OUTPUTS are for their rate and accuracy suitable for transmission of the measured data for further projection or directly into the control systems. We offer an isolated RS232 and RS485 with the ASCII/Modbus/PROFIBUS protocols and LAN.

MEASURED DATA RECORD is an internal time control of data collection. It is suitable where it is necessary to register measured values. Two modes may be used. FAST is designed for fast storage (80 records/s) of all measured values up to 8 000 records. Second mode is RTC, where data record is governed by Real Time with data storage in a selected time segment and cycle. Up to 266 000 values may be stored in the instrument memory. Data transmission into PC via serial interface RS 232/485 and OM Link.

STANDARD FUNCTIONS

PROGRAMMABLE INPUT

Selection: of input type and measuring range

Standard setting: any display values can be assigned to Min and Max values of a defined standard input signal

Teach-in: any display values can be assigned to Min and Max values of actual (unknown) input signal

Manual setting: known Min and Max input signal values can be entered manually and any display values can be assigned to each signal

EXCITATION

Range: 24 VDC/1 W, isolated

COMPENSATION

Wiring (RTD, OHM): automatic (3- or 4-wire) or manual in menu (2-wire)

Probes (RTD): internal wiring (resistance of conductors in the measuring head)

CJC (T/C): manual or automatic (terminal temperature)

FUNCTIONS

Linearization: non-linear signal is converted by a 177-point linear interpolation

Tare: designed to reset display upon non-zero input signal

Min./max. value: registration of min./max. value reached during measurement

Peak value: the display shows only max. or min. value

Mathemat. operations: polynom, 1/x, logarithm, exponential, power, root, sin x and operations between inputs

DIGITAL FILTERS

Floating / Exponential / Arithmetic average: from 2 to 100 measurements

Rounding: setting the display step for the display

EXTERNAL CONTROL

Hold: display/instrument blocking

Lock: control keys blocking

Tare: activation and tare resetting

Resetting Min/Max: resetting min/max value

TECHNICAL DATA

INPUT		PROJECTION	
No. of inputs	1 or 2 The range is adjustable in the instrument menu	Display	2x 99..999 LCD with backlighting
DC Range	±90/180 mA < 200 mV ±30/60 mV > 10 MΩ ±1000 mV > 10 MΩ ±20/40/80 V 1.25 MΩ	Input 1	
PM Range	±5/±20 mA < 400 mV 4...20 mA < 400 mV ±2/5/10 V 1 MΩ	Input 1 Input 1 Input 2	
OHM Range	0...15/30/50/100 Ω 0...1/3/15 kΩ 0...30 kΩ (only for 2- or 4-wire connection)	Input 3	
Connection	2, 3- and 4-wire	Input 2	
RTD Range	Pt 100/500/1000, 3,850 ppm/°C Pt 100, 3,920 ppm/°C Pt 50, 3,910 ppm/°C Pt 100, 3,910 ppm/°C	-50°...450°C -50°...450°C -200°...1100°C -200°...450°C	
Connection	2, 3- and 4-wire	RTD	
Ni Range	Ni 1000/10 000, 5 000 ppm/°C Ni 1000/10 000, 6 180 ppm/°C	-50°...250°C -200°...250°C	
Connection	2, 3- and 4-wire		
Cu Range	Cu 50/100, 4 260 ppm/°C Cu 50/100, 4 280 ppm/°C	-50°...200°C -200°...200°C	
Connection	2, 3- and 4-wire		
T/C Range	J (Fe-CuNi) K (NiCr-Ni) T (Cu-CuNi) E (NiCr-CuNi) B (PtRh30-PtRh6) S (PtRh10-Pt) R (Pt13Rh-Pt) N (Omega/galloy) L (Fe-CuNi)	-200°...900°C -200°...1300°C -200°...400°C -200°...690°C 300°...1820°C -50°...1760°C -50°...1740°C -200°...1300°C -200°...900°C	
CJC	adjustable -20°...99°C or automatical		
DU Sensor power supply	2 VDC/4 mA, potentiometer resistance > 500 Ω		

EXTERNAL INPUT	
No. of inputs	2, on contact or 24 V
Function	No function assigned Activation of Tare Reset of Tare Measurement paused Resetting min/max value Device buttons blocked Resetting and preset of counter/clock Sum showing Sum reset Data recording start (RTC) Data recording reset (RTC) Value display „Math. functions“

PROJECTION	
Display	2x 99..999 LCD with backlighting
Description	2x 3 characters on the display may be used for description of measured quantities
Decimal point	adjustable - in menu

INSTRUMENT SPECIFICATION	
TC	50 ppm/°C
Accuracy	±0.15% of FS ±0.25% of FS Ni 1000TD ±0.3% of FS T/C above accuracies apply for projection 9999 and 10 meas./s
Rate	0.5...80 measurement/s
Overload	10x (t < 30 ms), 2x
Compensation of conduct	< 30 Ω
Measurement accuracy CJC	±1.5°C
Functions	offset, Min/max value, Tare, peak value, math. functions
Digital filters	exponential / floating / arithmetic average, rounding
Math functions	polynomial / inverse polynomial / logarithm / exponential / power / root
Linearization	linear interpolation in 177 points and 3 tables setup only via OM Link
Measured data logging	RTC time-date-display value < 266 000 records FAST: display value < 8 000 records
OM Link	company communication interface for operation, setting and update of instruments (microUSB)
Watch-dog	reset after 400 ms
Calibration	at 25°C and 40% r.h.

RELAYS / OC OUTPUT	
No. of outputs	up to 6
Type	digital, menu adjustable
Mode	HYSTER. active above set value WINDOW active in the set window / band BATCH active in set period
Function Relays/OC	CLOSE is closed in active mode OPEN is open in active mode
Limits	-99999...99999
Hysteresis	0...99999
Delay	0...99.9 s
Outputs	1...6x relay with switching contact (Form C) (250 VAC/50 VDC, 3 A)* 1...6x open collector (30 VDC/100 mA)
Relays	1/8 HP 277 VAC, 1/10 HP 125 V, Pilot Duty D300


* values apply for resistance load

ANALOG OUTPUTS	
No. of outputs	up to 4
Type	isolated, adjustable with 16-bit DAC, output type and range is selectable
TC	15 ppm/°C
Accuracy	±0.025% of FS ±0.03% of FS ±0.06% of FS 0.5 V 0.2 V / 0.5 mA
Rate	response to change of value < 1 ms
Ranges	0...2 / 5 / 10 V, ±10 V, resistive load > 1 kΩ 0...5 / 20 mA / 4...20 mA, comp. < 600 Ω / 12 V Indication of error message (output < 3.2 mA)

DATA OUTPUTS	
No. of outputs	up to 2
Protocol	ASCII, MESSBUS, Modbus RTU, PROFIBUS DP
Data format	8 bit + no parity + 1 stop bit (ASCII) 7 bit + even parity + 1 stop bit (Modbus)
Rate	300...230 400 Baud 9 600 Baud...12 Mbaud (PROFIBUS)
RS 232	isolated
RS 485	isolated, addressing (max. 31 instruments)
Ethernet	10/100BaseT, TCP/IP Modbus (Slave)

EXCITATION	
Fixed	24 VDC, < 1 W, isolated

CONNECTION

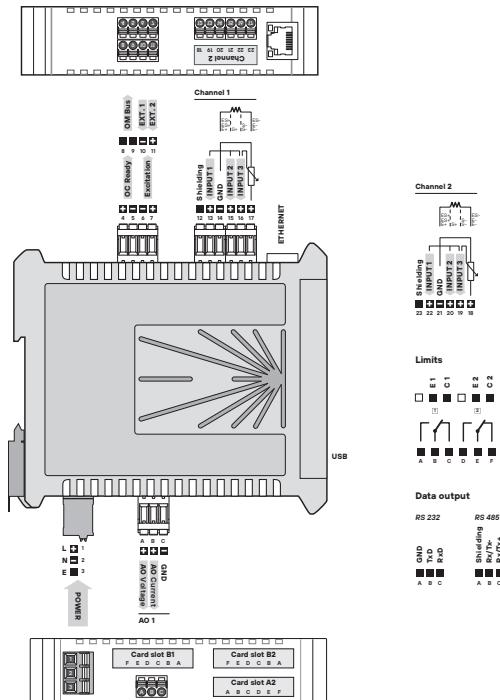

ORDER CODE

OMX 103UNI

-	□□□	-	□□□	-	□
Power supply	10...30 VDC / 24 VAC 80...250 V AC/DC	0 1	A B		
Number inputs	1 input 2 inputs		0 1		
Analogue output	no yes			0 1	
Card A2	no Comparator - 2x relays Comparator - 2x open collectors Analogue output RS 232 RS 485 PROFIBUS			0 1 2 3 4 5 6	
Card B1	no Comparator - 2x relays Comparator - 2x open collectors Analogue output			0 1 2 3	
Card B2	no Comparator - 2x relays Comparator - 2x open collectors Analogue output RS 232 RS 485			0 1 2 3 4 5	
Ethernet - TCP/IP Modbus	no yes			0 1	
Data record	no yes			0 1	
Specification	customized version, do not fill in			00	

Basic configuration of the instrument is indicated in bold.